

Sample Name :Systemin
 Cat. No. :RP10622-0.5
 Lot. No. :PE5481902;
 Time Processed : 10:24:58
 Month-Day-Year Processed : 02/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 27.00 | Pumps | Pump B Conc. | 95 | |
| 27.01 | Pumps | Pump B Conc. | 5 | |
| 35.00 | Pumps | Pump B Conc. | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

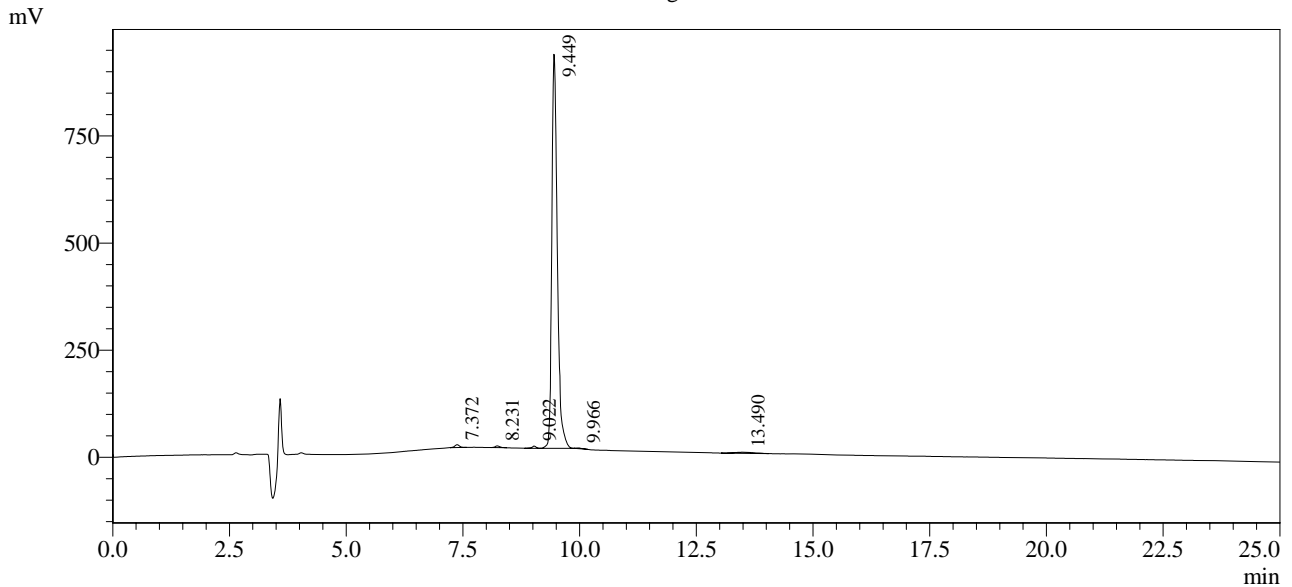

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 7.372 | 45811 | 6607 | 0.592 |
| 2 | 8.231 | 28157 | 3972 | 0.364 |
| 3 | 9.022 | 34340 | 5336 | 0.443 |
| 4 | 9.449 | 7547334 | 919936 | 97.465 |
| 5 | 9.966 | 12342 | 1417 | 0.159 |
| 6 | 13.490 | 75628 | 2580 | 0.977 |
| Total | | 7743612 | 939847 | 100.000 |