

Sample Name :-Amyloid (1-40)
 Cat. No. : RP20528
 Lot. No. : PE1871811
 Time Processed : 13:27:11
 Month-Day-Year Processed : 11/24/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

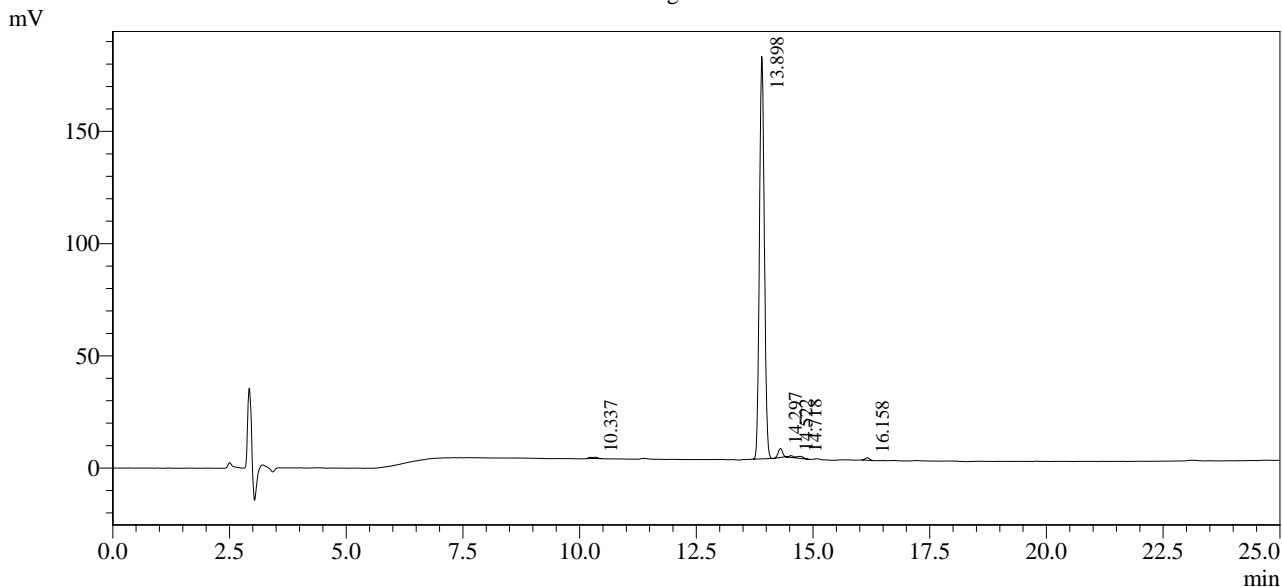

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.337	5418	545	0.397
2	13.898	1311555	179376	96.160
3	14.297	26548	4038	1.946
4	14.522	4780	763	0.350
5	14.718	8768	904	0.643
6	16.158	6864	1084	0.503
Total		1363934	186709	100.000