

Sample Name :Bacterial Sortase Substrate III, Abz/DNP
 Cat. No. : RP20431
 Lot. No. :E4962119I
 Time Processed :2:07:38
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

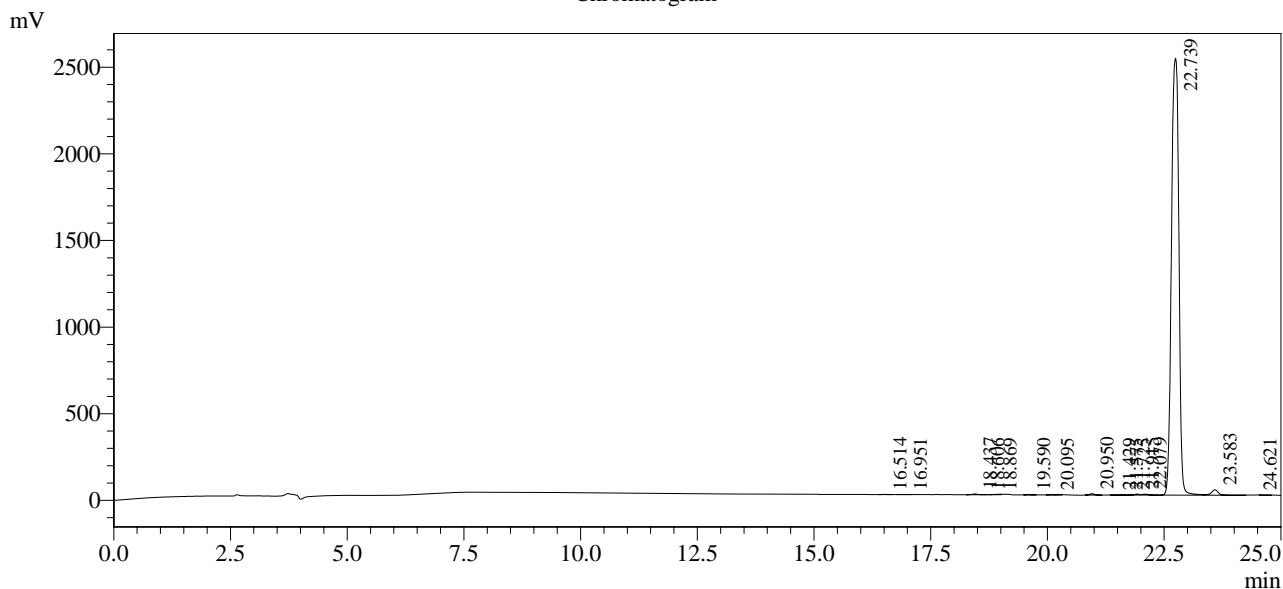

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.514	3723	492	0.013
2	16.951	3982	426	0.014
3	18.437	27171	4085	0.096
4	18.606	5766	870	0.020
5	18.869	2293	358	0.008
6	19.590	3852	622	0.014
7	20.095	5338	695	0.019
8	20.950	50024	7892	0.177
9	21.429	2250	433	0.008
10	21.575	3770	526	0.013
11	21.725	3789	551	0.013
12	21.915	41442	5369	0.147
13	22.079	45998	5897	0.163
14	22.739	27752892	2521336	98.142
15	23.583	323177	30747	1.143
16	24.621	2911	448	0.010
Total		28278380	2580748	100.000