

Sample Name :Human Papillomavirus (HPV) E7 protein (49 - 57)
Cat. No. : RP20249
Lot. No. :PE6801704

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

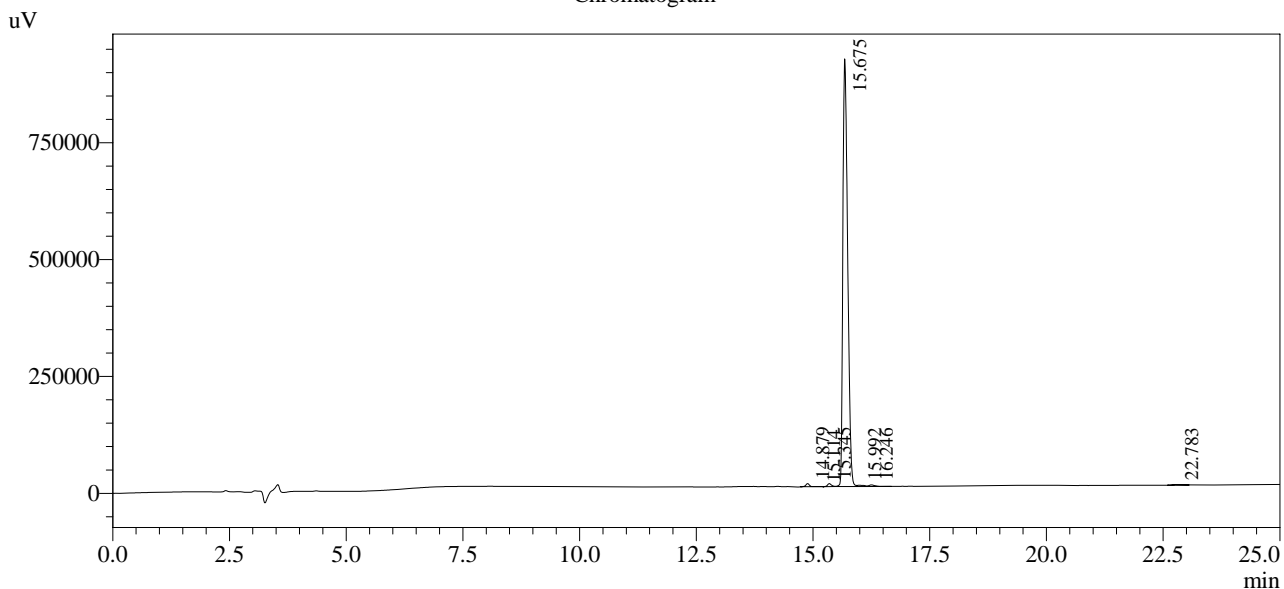

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.879	34753	6580	0.519
2	15.114	3202	410	0.048
3	15.345	38850	6349	0.580
4	15.675	6552466	915042	97.799
5	15.992	26744	2665	0.399
6	16.246	29720	3329	0.444
7	22.783	14205	1027	0.212
Total		6699939	935401	100.000