

Sample Name :c-Myc Peptide
 Cat No. :RP11731
 Lot No. :E7153020G
 Time Processed :10:23:06 AM
 Month-Day-Year Processed :07/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

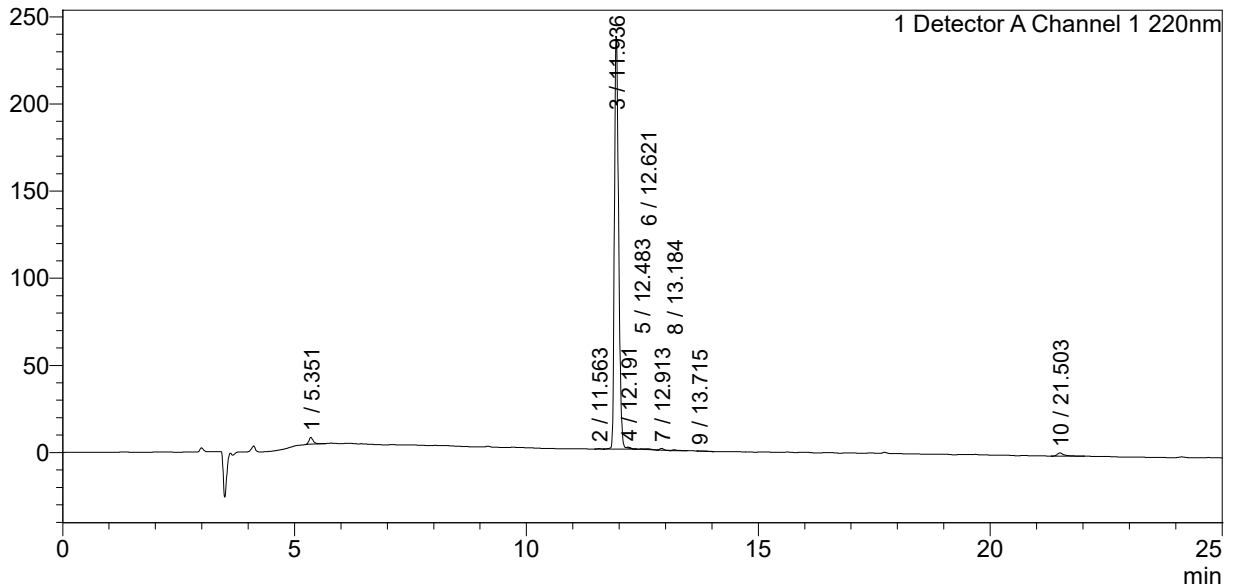

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.351	25271	3925	1.602
2	11.563	1851	339	0.117
3	11.936	1510425	237101	95.735
4	12.191	2442	430	0.155
5	12.483	2518	304	0.160
6	12.621	4342	517	0.275
7	12.913	5959	1063	0.378
8	13.184	3779	480	0.240
9	13.715	1356	59	0.086
10	21.503	19780	1808	1.254
Total		1577722	246027	100.000