

Sample Name :Kisspeptin-10
 Cat. No. : RP20494
 Lot. No. : PE6711710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

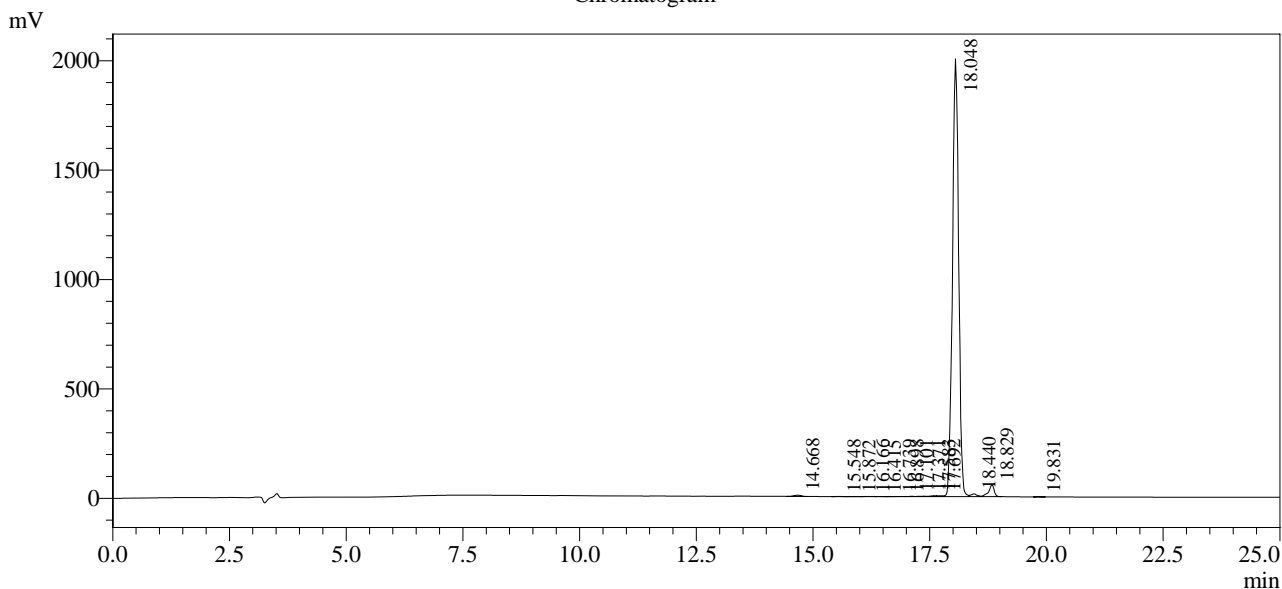

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.668	59990	5490	0.311
2	15.548	4961	756	0.026
3	15.872	1708	193	0.009
4	16.166	5403	765	0.028
5	16.415	1493	276	0.008
6	16.739	7277	715	0.038
7	16.898	4043	649	0.021
8	17.101	14024	1557	0.073
9	17.371	24418	2021	0.127
10	17.583	37162	4266	0.193
11	17.692	28795	4327	0.149
12	18.048	18550435	2001154	96.143
13	18.440	110108	12754	0.571
14	18.829	440449	54856	2.283
15	19.831	4336	692	0.022
Total		19294601	2090471	100.000