

Sample Name: OVA G4 peptide
 Cat No. : RP20398
 Lot No. : E90044720G
 Time Processed: 1:53:24 PM
 Month-Day-Year Processed : 07/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|----------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 0 |
| 25.00 | Pumps | Pump A B.Conc | 60 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Curve | 0 |
| 31.01 | Pumps | Pump A B.Conc | 0 |
| 40.00 | Pumps | Pump A B.Conc | 0 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

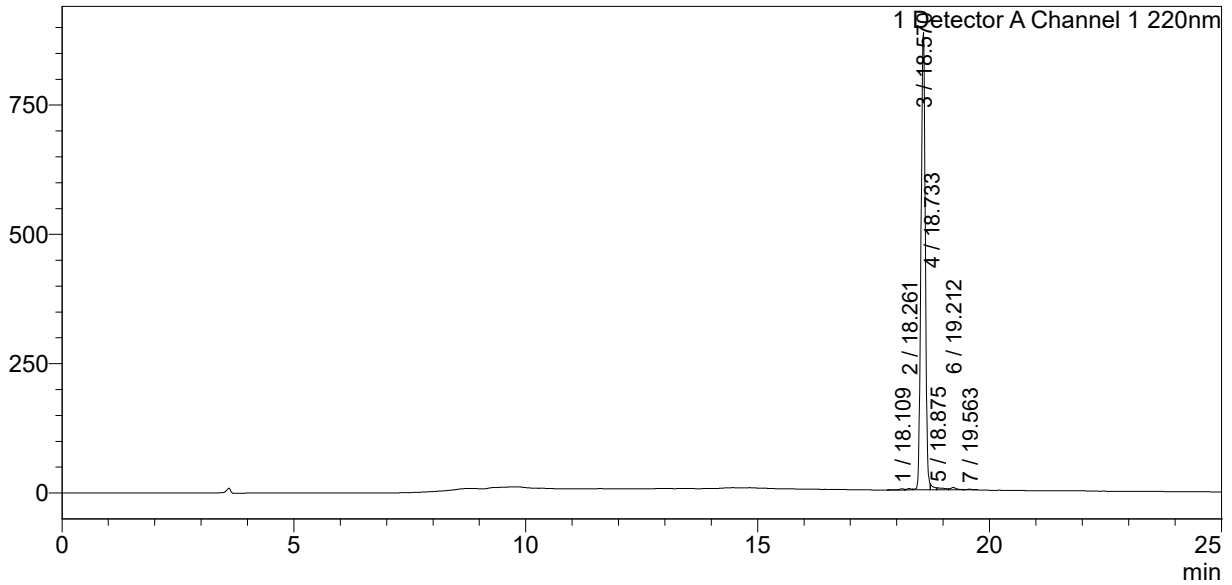

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 18.109 | 19100 | 2197 | 0.324 |
| 2 | 18.261 | 18257 | 2670 | 0.310 |
| 3 | 18.570 | 5710803 | 885077 | 96.832 |
| 4 | 18.733 | 50019 | 9910 | 0.848 |
| 5 | 18.875 | 45686 | 3735 | 0.775 |
| 6 | 19.212 | 43067 | 4634 | 0.730 |
| 7 | 19.563 | 10697 | 1379 | 0.181 |
| Total | | 5897628 | 909602 | 100.000 |