

Sample Name : β -Amyloid (1-15)
 Cat No. :RP20141
 Lot No. :E5051020F
 Time Processed :13:28:03
 Month-Day-Year Processed :06/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

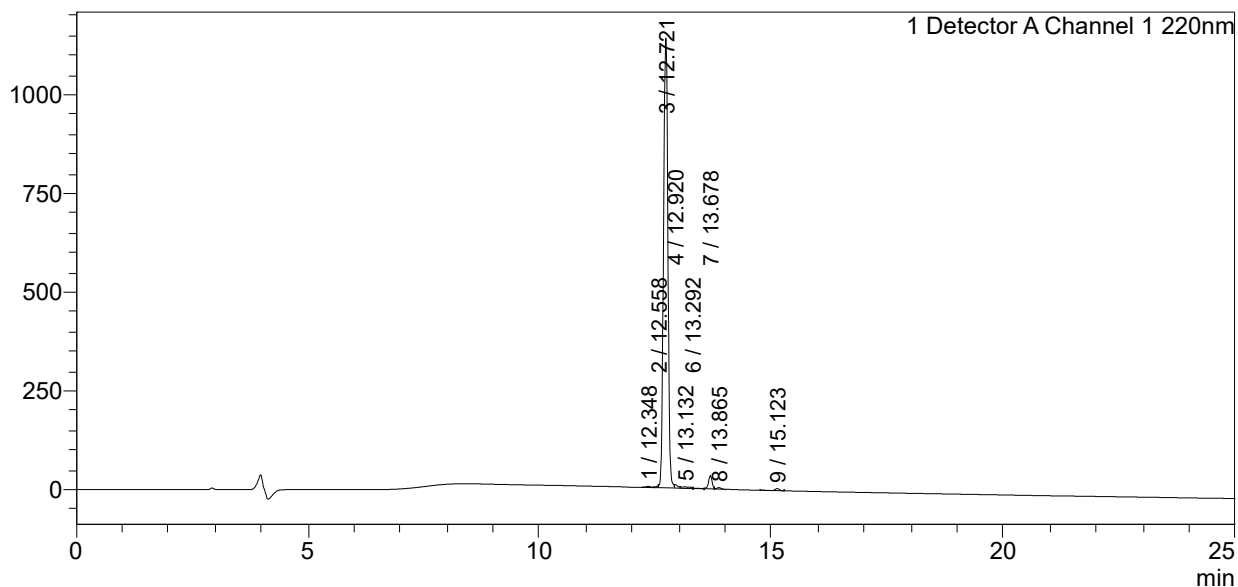

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.348	22430	3050	0.286
2	12.558	20840	5209	0.266
3	12.721	7449927	1138866	95.043
4	12.920	46564	8760	0.594
5	13.132	45011	3842	0.574
6	13.292	12812	1880	0.163
7	13.678	183334	33707	2.339
8	13.865	23710	3839	0.302
9	15.123	33844	5468	0.432
Total		7838473	1204621	100.000