

Sample Name :Somatostatin
 Cat No.: RP10226
 Lot No.:E6035620C
 Time Processed :8:32:04
 Month-Day-Year Processed :04/04/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

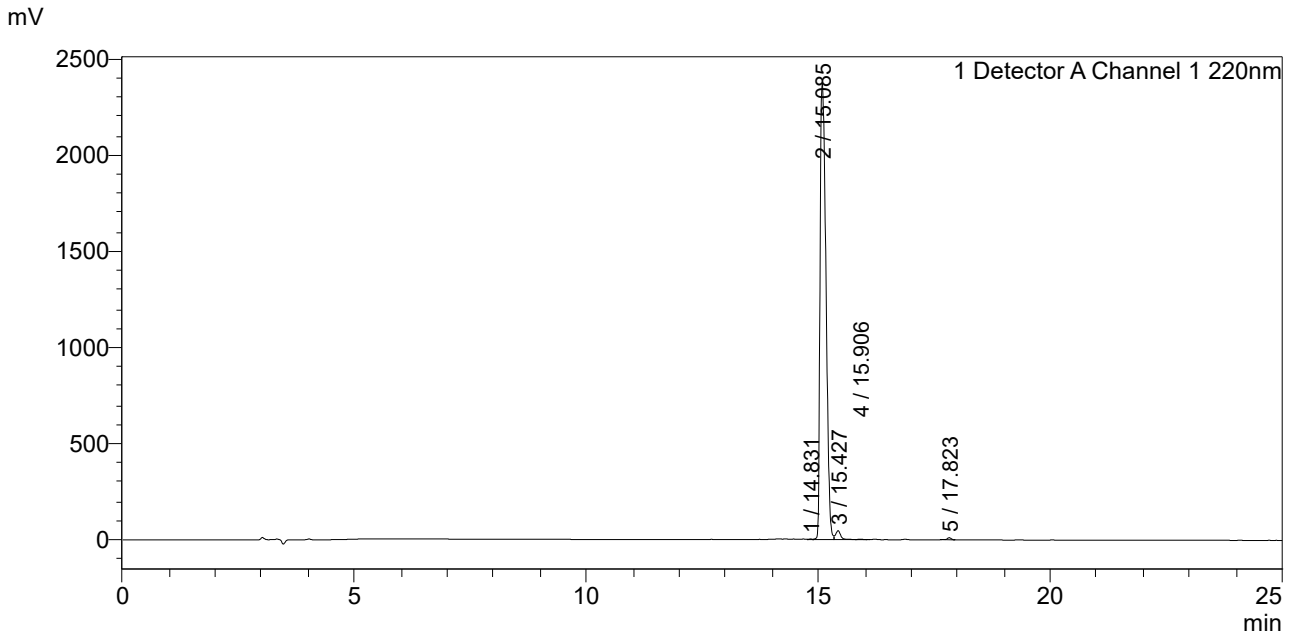

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.831	20726	3111	0.097
2	15.085	20984314	2373168	97.846
3	15.427	365558	46978	1.705
4	15.906	13156	2168	0.061
5	17.823	62604	10686	0.292
Total		21446358	2436111	100.000