

Sample Name :Endomorphin-1
 Cat No. :RP10925
 Lot No. :E6868520H
 Time Processed :5:01:06
 Month-Day-Year Processed :08/06/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

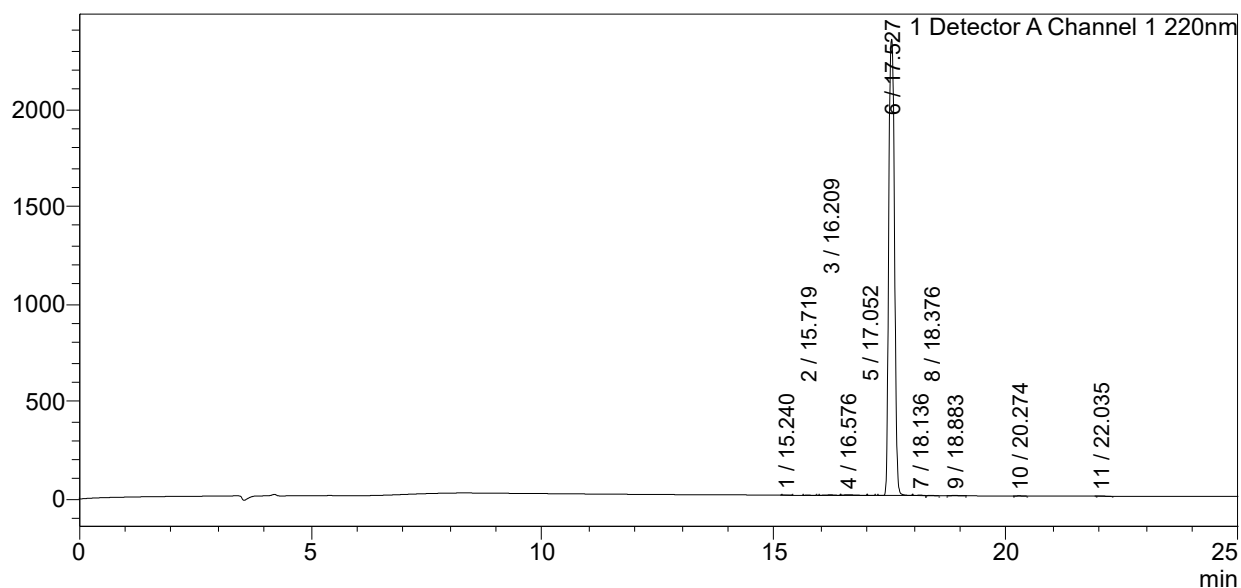

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.240	2944	484	0.015
2	15.719	3518	428	0.017
3	16.209	35534	2840	0.177
4	16.576	54173	2830	0.269
5	17.052	1377	240	0.007
6	17.527	19961679	2341828	99.212
7	18.136	19480	2512	0.097
8	18.376	10052	1565	0.050
9	18.883	22790	2869	0.113
10	20.274	5977	898	0.030
11	22.035	2632	285	0.013
Total		20120157	2356780	100.000