


Mass Spectrum

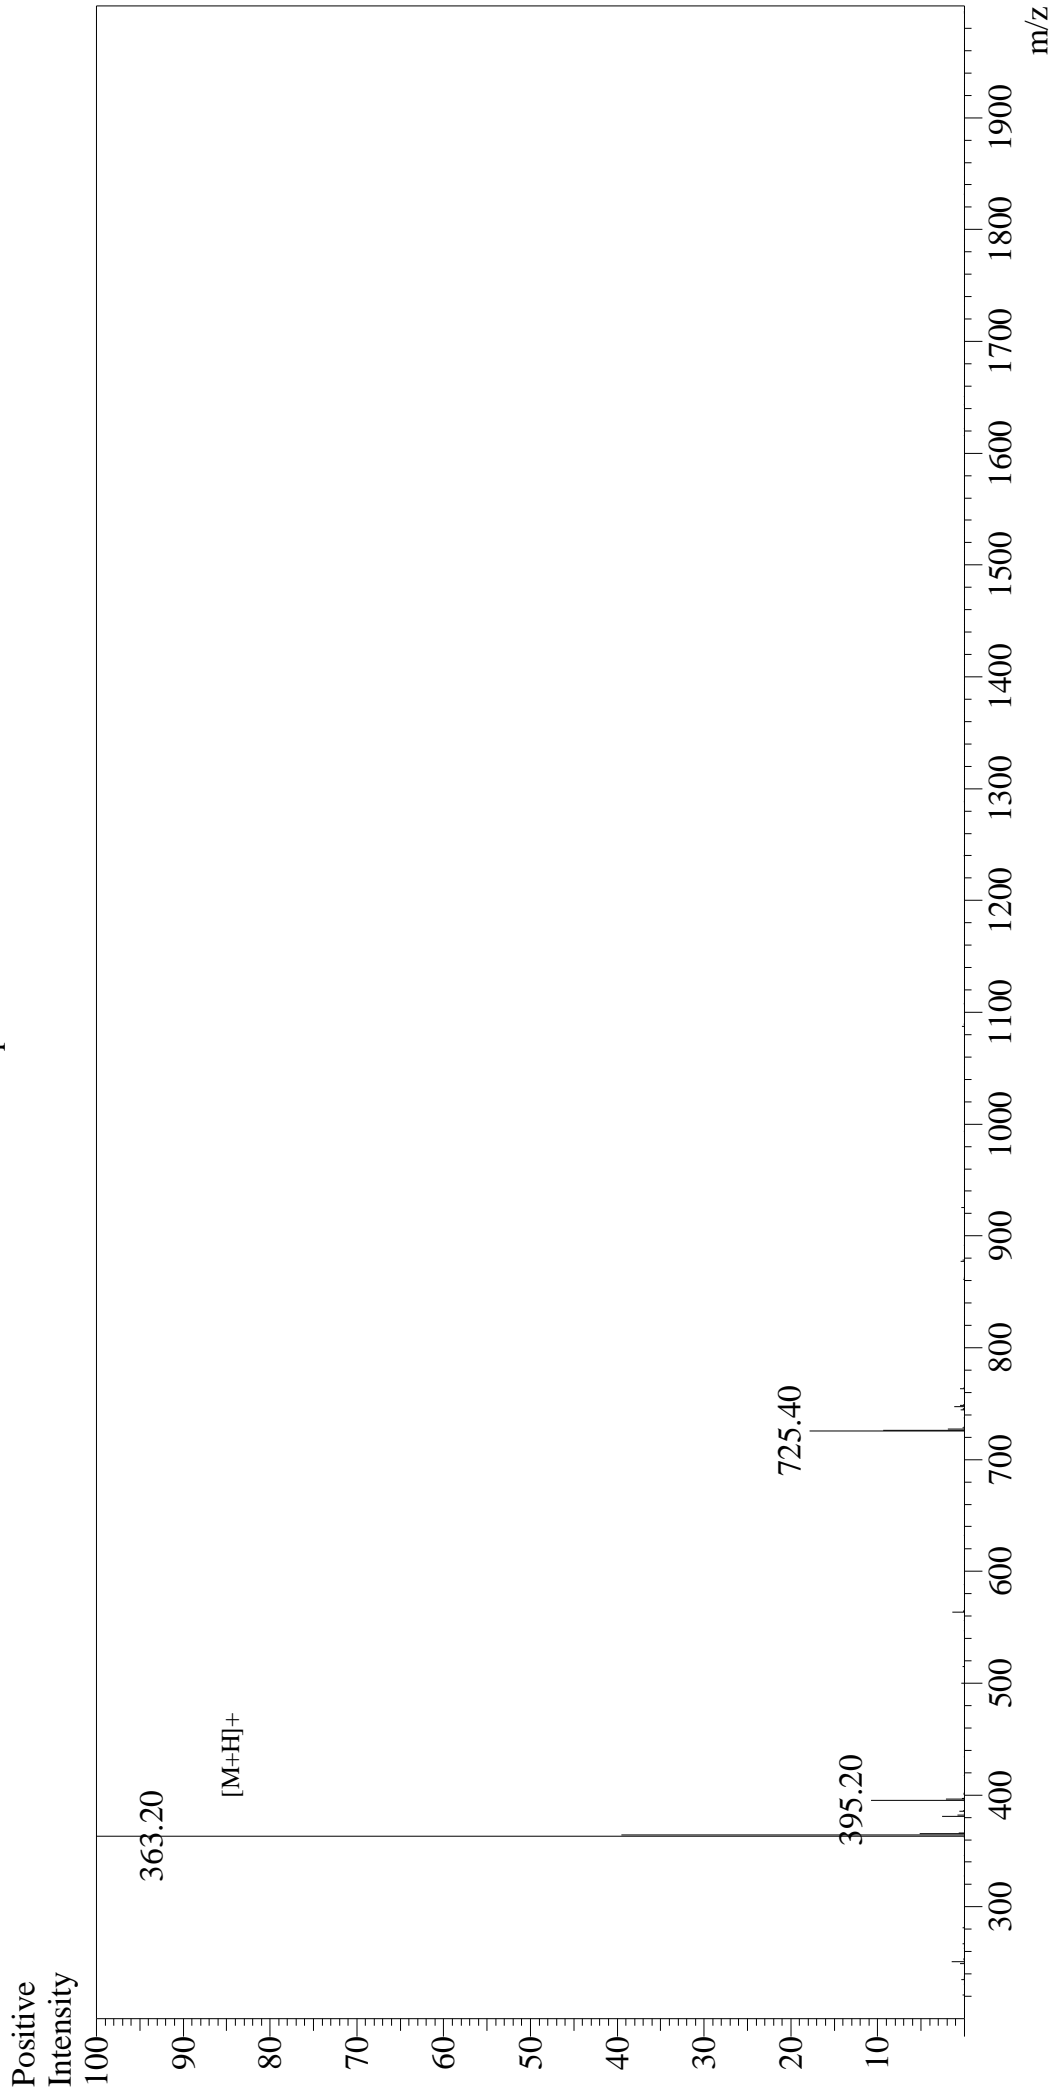

Sample Information

User : Gary
Month-Day Processed : 10/15/17
Time Processed : 16:09:41
Injection Volume : 0.2
Sample Name : Thyrotropin-Releasing Hormone (TRH)
Cat No. : RP10112
Lot No. : PE1071710
Theoretical MW : 362.38
Observed MW : 362.20

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH