

Sample Name :β-Amyloid (22-35)
 Cat No: RP20130
 Lot No : E4711120K
 Time Processed :12:52:43 AM
 Month-Day-Year Processed :11/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
41.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

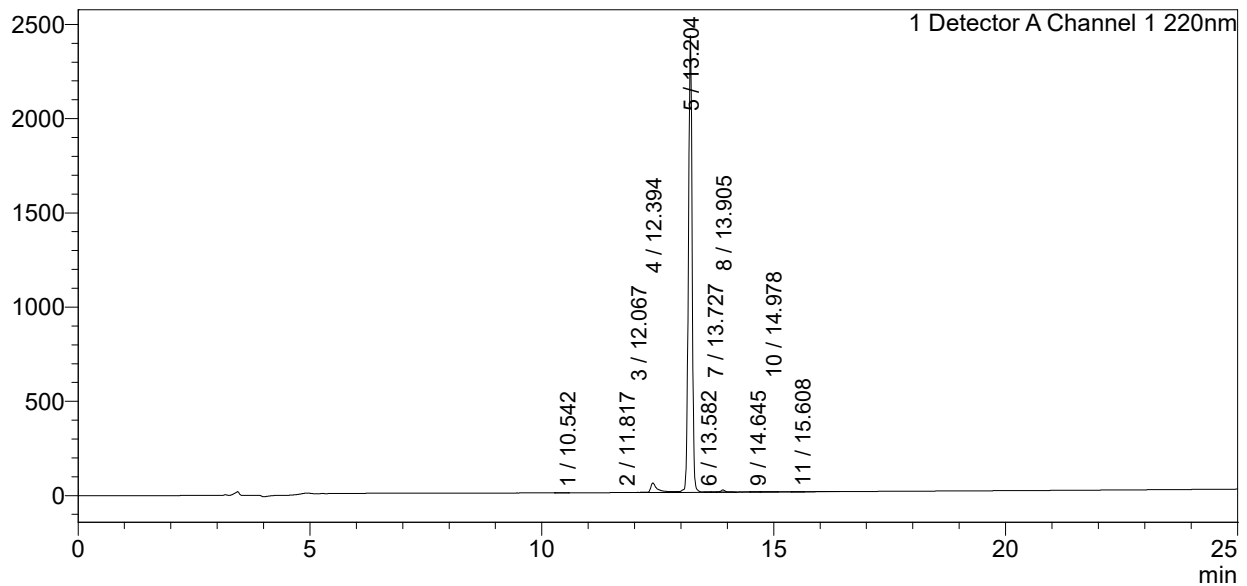

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.542	1001	90	0.007
2	11.817	9878	1193	0.070
3	12.067	13785	1027	0.098
4	12.394	543296	50310	3.858
5	13.204	13418544	2423595	95.294
6	13.582	5378	1251	0.038
7	13.727	6625	1206	0.047
8	13.905	74275	11477	0.527
9	14.645	1469	211	0.010
10	14.978	5902	734	0.042
11	15.608	1107	62	0.008
Total		14081260	2491157	100.000