

Sample Name :Cortistatin 14, human, rat
 Cat No. : RP10972
 Lot No. : PE2251903
 Time Processed : 23:25:40
 Month-Day-Year Processed : 03/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

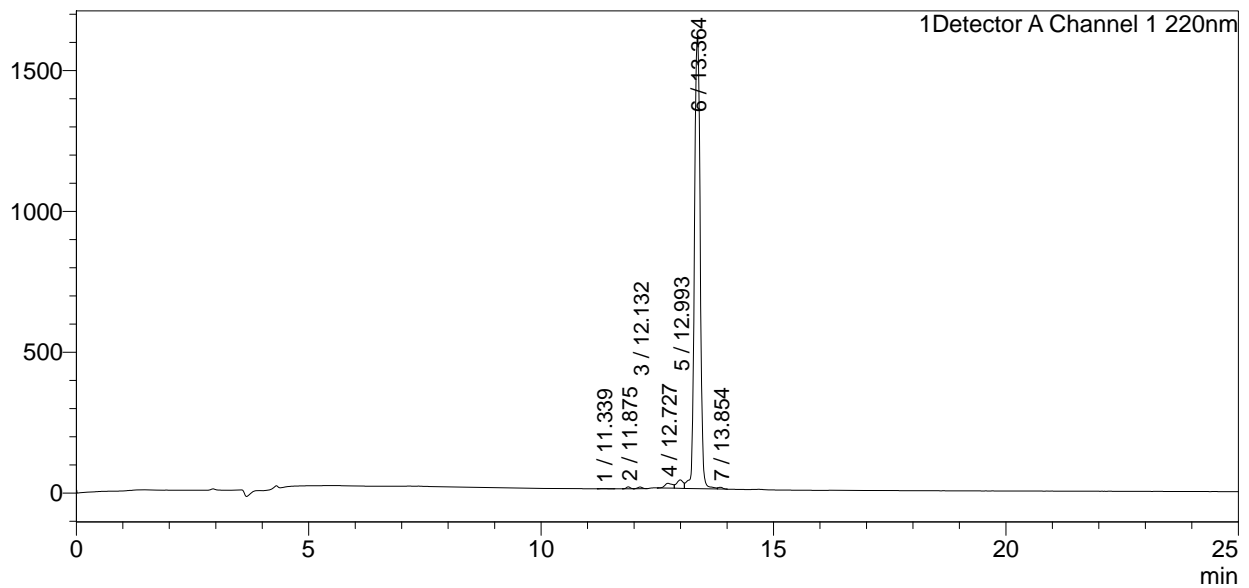

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.339	8323	805	0.058
2	11.875	41068	7068	0.285
3	12.132	42771	6203	0.297
4	12.727	200473	17151	1.391
5	12.993	292410	30033	2.029
6	13.364	13784869	1604882	95.642
7	13.854	43054	6314	0.299
Total		14412968	1672456	100.000