

Sample Name :Influenza Hemagglutinin (307-319)  
 Cat No: RP20087  
 Lot No : E4296921D

Time Processed :22:48:52  
 Month-Day-Year Processed :04/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

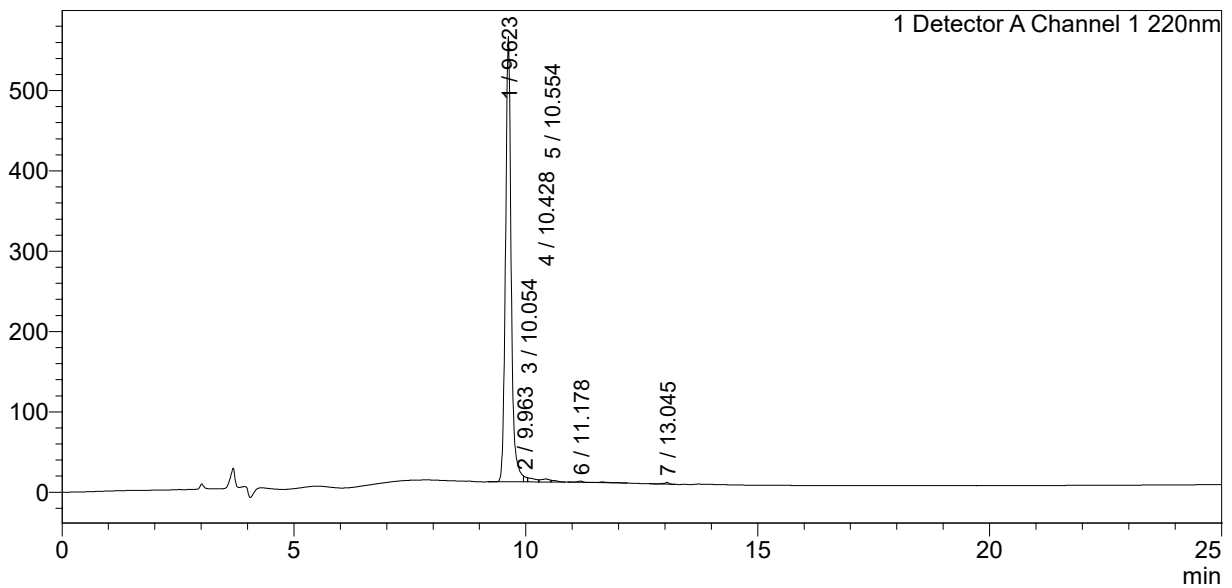

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.623	4714947	554633	96.098
2	9.963	32092	6923	0.654
3	10.054	54559	4993	1.112
4	10.428	47587	3723	0.970
5	10.554	17790	2064	0.363
6	11.178	24236	1641	0.494
7	13.045	15201	2198	0.310
Total		4906412	576175	100.000