

Sample Name :Physalaemin  
 Cat No :RP10474  
 Lot No :E6525720J;  
 Time Processed :8:11:17 AM  
 Month-Day-Year Processed :10/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

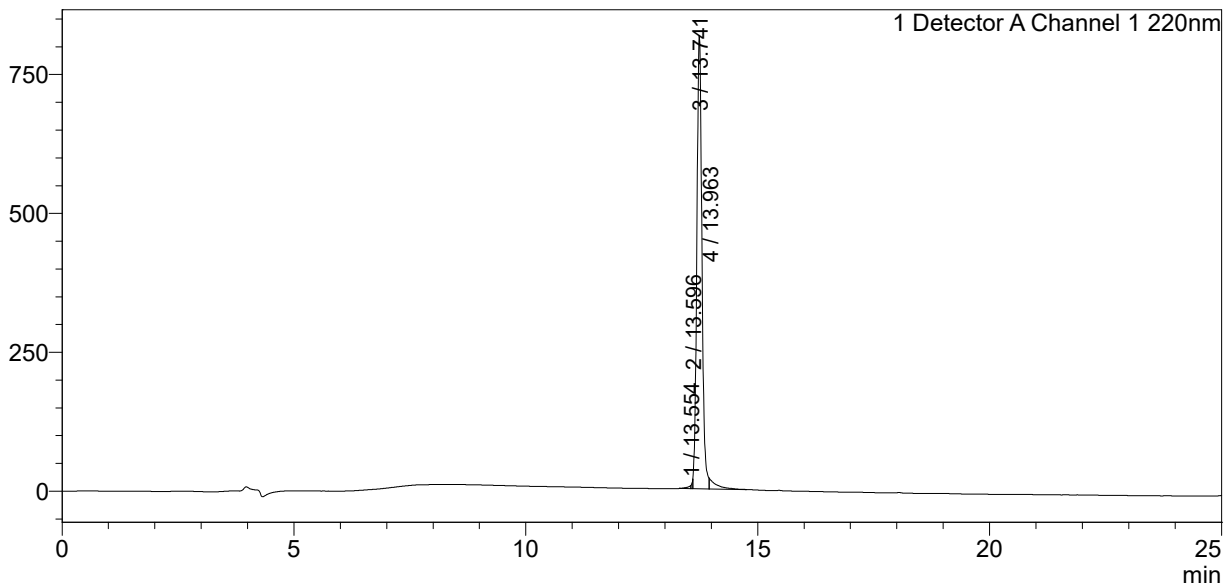

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.554	29186	5001	0.448
2	13.596	27276	12893	0.419
3	13.741	6259323	815955	96.104
4	13.963	197296	18700	3.029
Total		6513081	852549	100.000