

Sample Name :GRGDSP  
 Cat. No. : RP20255  
 Lot. No. : E1353620A  
 Time Processed :8:23:39  
 Month-Day-Year Processed : 01/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

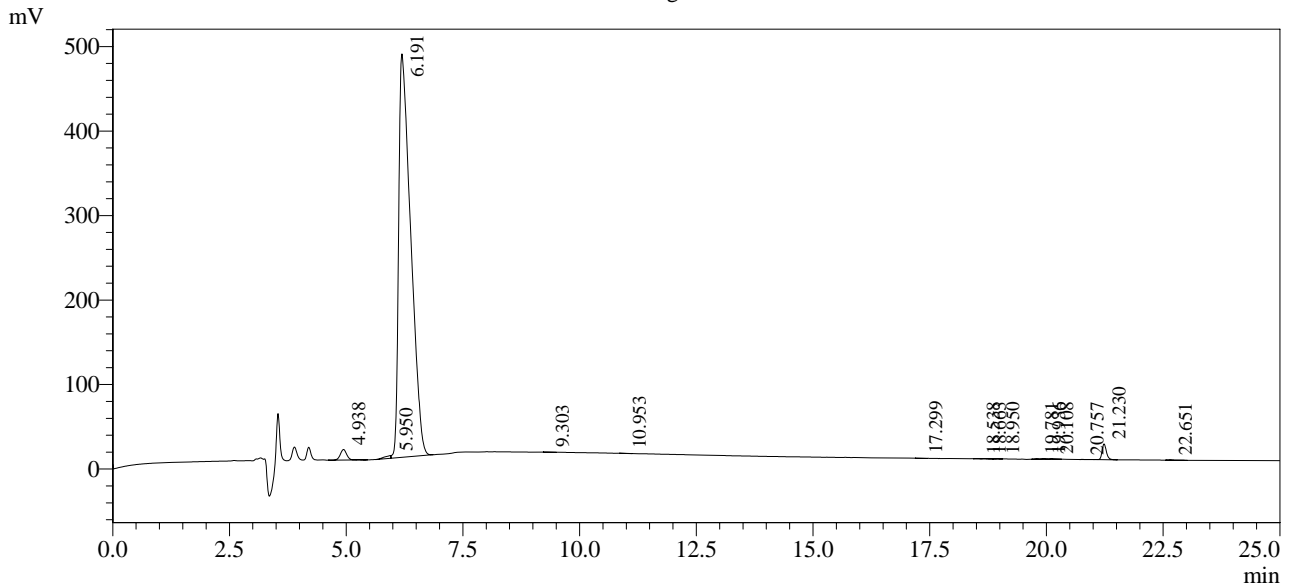

1 Det.A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.938	121447	12583	1.371
2	5.950	32402	3158	0.366
3	6.191	8557247	477455	96.593
4	9.303	1688	289	0.019
5	10.953	1534	243	0.017
6	17.299	1419	197	0.016
7	18.538	1696	288	0.019
8	18.663	2500	350	0.028
9	18.950	1562	190	0.018
10	19.781	3276	526	0.037
11	19.936	4813	645	0.054
12	20.108	4363	538	0.049
13	20.757	1116	118	0.013
14	21.230	121127	18752	1.367
15	22.651	2864	311	0.032
Total		8859055	515644	100.000