

Sample Name :Gastrin-Releasing Peptide, human  
 Cat No. :RP10791  
 Lot No. :E2869221E  
 Time Processed :4:26:57 PM  
 Month-Day-Year Processed :05/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

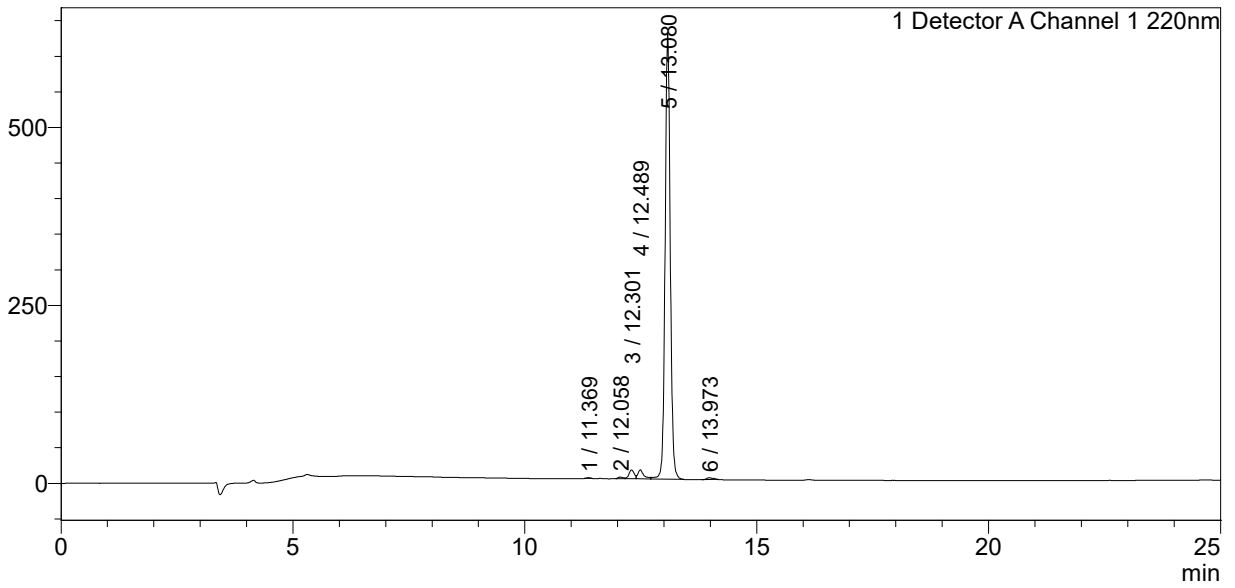

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.369	5393	1097	0.106
2	12.058	15071	2068	0.295
3	12.301	96333	12413	1.886
4	12.489	109491	12600	2.144
5	13.080	4856507	626086	95.092
6	13.973	24345	2533	0.477
Total		5107140	656797	100.000