

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10610
 Lot No. :E8093821C
 Time Processed :11:25:51 PM
 Month-Day-Year Processed :03/12/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

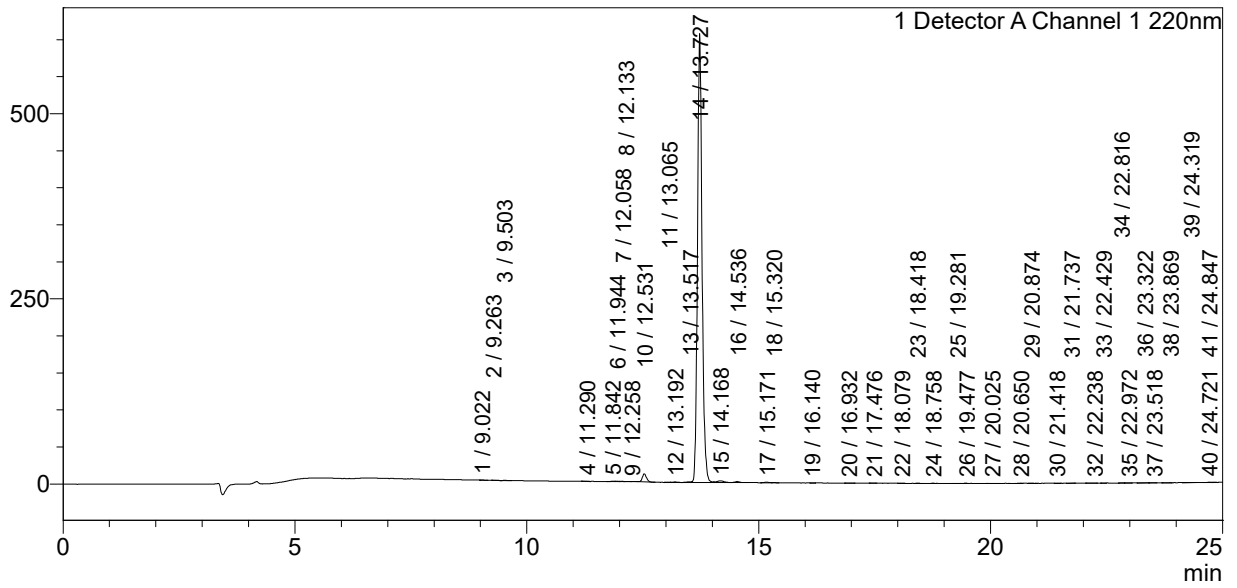

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.022	1013	157	0.023
2	9.263	1696	189	0.039
3	9.503	1413	197	0.033
4	11.290	1439	273	0.033
5	11.842	3037	423	0.070
6	11.944	1962	465	0.045
7	12.058	2265	384	0.052
8	12.133	2109	308	0.049
9	12.258	1039	260	0.024
10	12.531	69403	11083	1.606
11	13.065	1412	240	0.033
12	13.192	4069	609	0.094
13	13.517	5831	857	0.135
14	13.727	4151159	606120	96.081

Peak#	Ret. Time	Area	Height	Area%
15	14.168	22295	2070	0.516
16	14.536	8899	1179	0.206
17	15.171	5533	664	0.128
18	15.320	1516	279	0.035
19	16.140	1158	221	0.027
20	16.932	1390	192	0.032
21	17.476	1090	185	0.025
22	18.079	1349	179	0.031
23	18.418	1518	244	0.035
24	18.758	1178	263	0.027
25	19.281	1335	169	0.031
26	19.477	1673	282	0.039
27	20.025	1299	158	0.030
28	20.650	1153	199	0.027
29	20.874	1268	165	0.029
30	21.418	1189	175	0.028
31	21.737	1423	183	0.033
32	22.238	2010	211	0.047
33	22.429	1334	224	0.031
34	22.816	1345	223	0.031
35	22.972	1011	175	0.023
36	23.322	2864	248	0.066
37	23.518	1056	169	0.024
38	23.869	1274	185	0.029
39	24.319	3298	301	0.076
40	24.721	1880	291	0.044
41	24.847	1297	230	0.030
Total		4320484	630631	100.000