

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat No. :RP11110
 Lot No. :E9391021G
 Time Processed : 2:33:36 PM
 Month-Day-Year Processed : 07/22/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

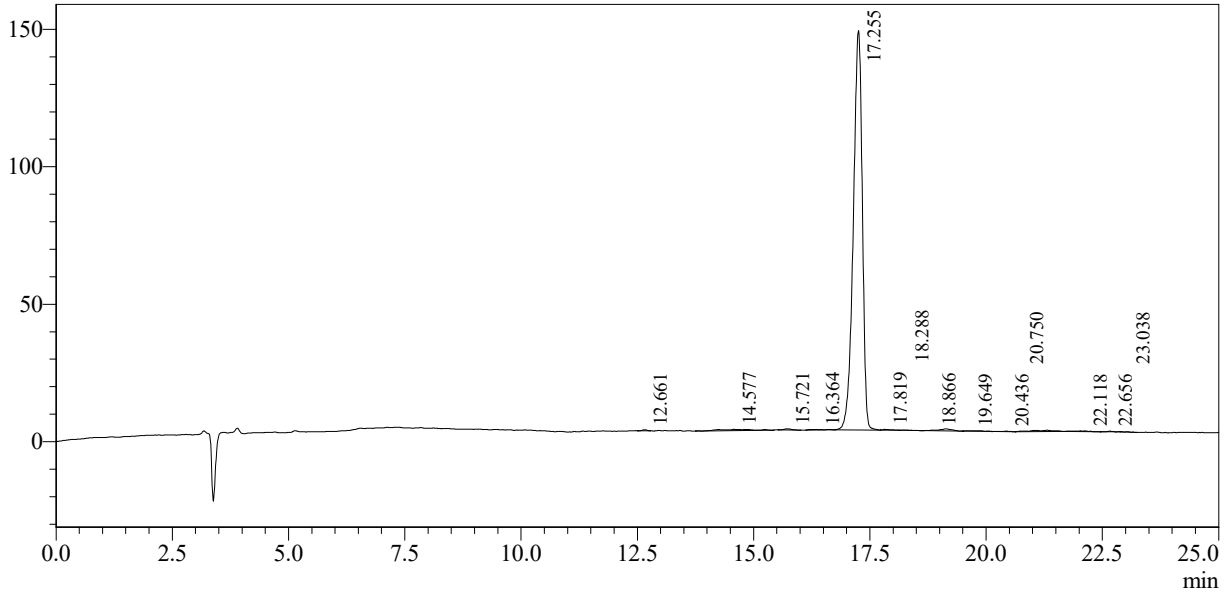

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.661	2238	377	0.110
2	14.577	22829	469	1.121
3	15.721	4801	433	0.236
4	16.364	4533	204	0.223
5	17.255	1955821	143588	96.077
6	17.819	2990	261	0.147
7	18.288	922	84	0.045
8	18.866	14053	250	0.690
9	19.649	3908	178	0.192
10	20.436	1183	162	0.058
11	20.750	15872	244	0.780
12	22.118	5060	242	0.249
13	22.656	894	183	0.044
14	23.038	569	107	0.028
Total		2035676	146781	100.000