

Sample Name :Somatostatin
Cat No.: RP10226
Lot No.: E8852520D
Time Processed :7:45:57
Month-Day-Year Processed :05/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment:ZJ19010014

<Chromatogram>

mV

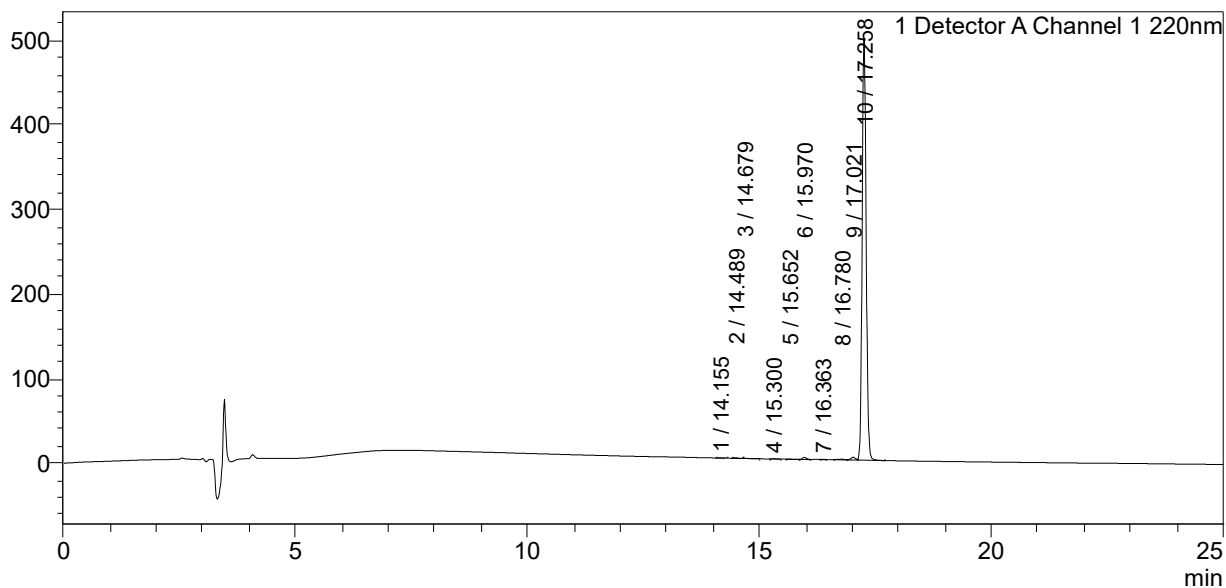

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.155	1110	208	0.037
2	14.489	4407	828	0.145
3	14.679	1052	104	0.035
4	15.300	1823	330	0.060
5	15.652	1283	185	0.042
6	15.970	14658	2460	0.483
7	16.363	1619	357	0.053
8	16.780	7891	831	0.260
9	17.021	21817	3326	0.719
10	17.258	2977636	499729	98.165
Total		3033296	508358	100.000