

Sample Name :Neuropeptide Y(1-36)  
 Cat No. :RP20520  
 Lot No. : E4942896I  
 Time Processed : 23:39:46  
 Month-Day-Year Processed : 09/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

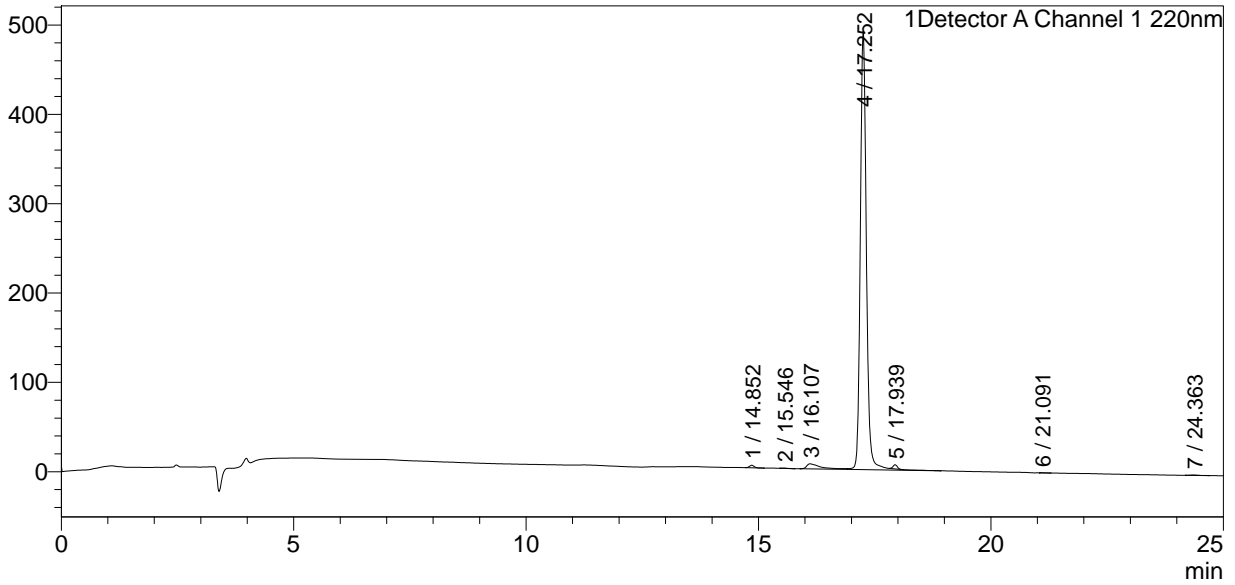

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.852	19093	2810	0.411
2	15.546	2349	318	0.051
3	16.107	122672	5675	2.640
4	17.252	4467145	490399	96.126
5	17.939	29576	4671	0.636
6	21.091	1193	144	0.026
7	24.363	5151	443	0.111
Total		4647178	504461	100.000