

Sample Name :Angiotensin I, human
 Cat No. :RP11251
 Lot No. :PE8995020F
 Time Processed :5:38:21
 Month-Day-Year Processed :06/05/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

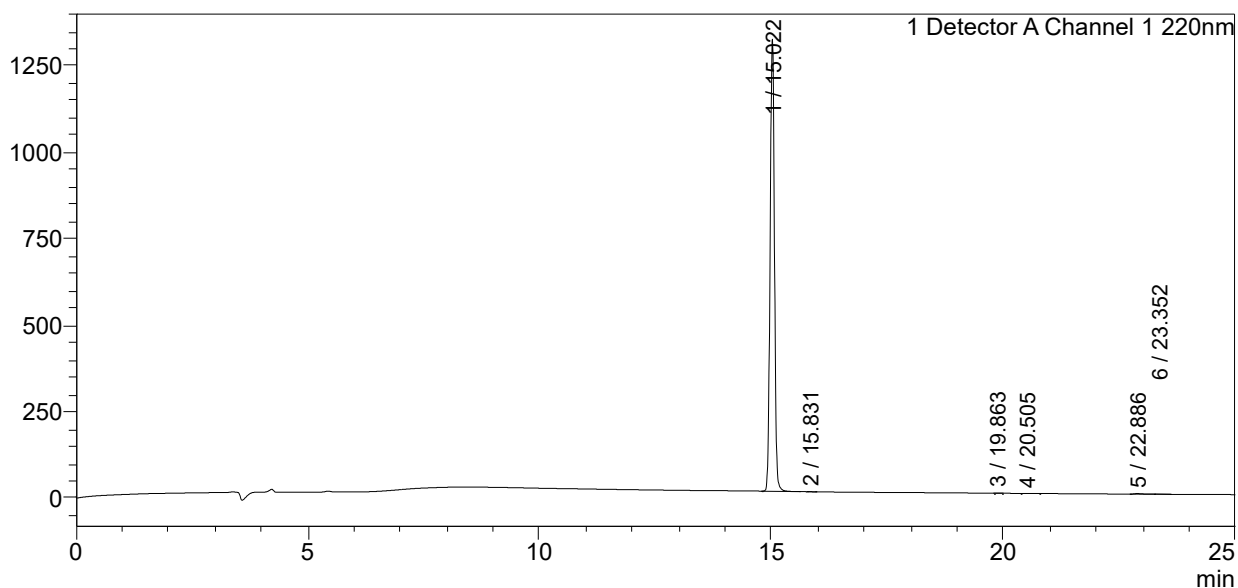

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.022	8435092	1308214	99.724
2	15.831	1636	249	0.019
3	19.863	1535	282	0.018
4	20.505	3071	199	0.036
5	22.886	15796	1577	0.187
6	23.352	1318	144	0.016
Total		8458447	1310665	100.000