

Sample Name : Octreotide (SMS 201-995)
 Cat. No. : RP10222
 Lot. No. : PE7451902
 Time Processed : 6:56:01
 Month-Day-Year Processed : 03/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

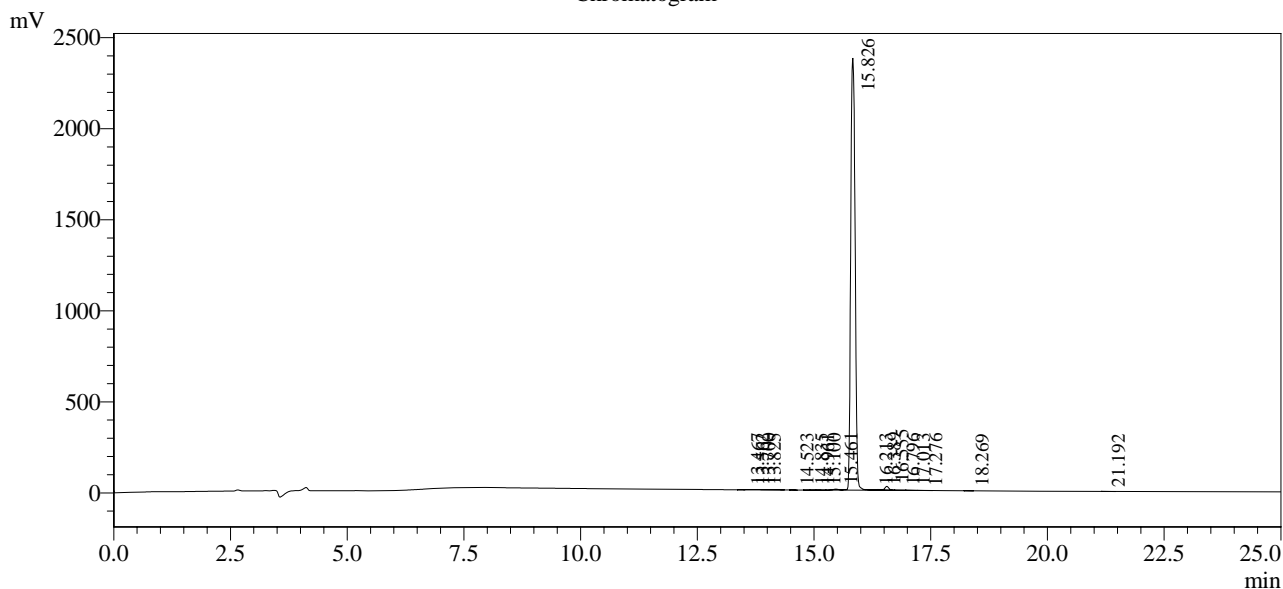

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.467	2329	354	0.015
2	13.562	2865	541	0.018
3	13.700	8324	730	0.053
4	13.825	14585	713	0.092
5	14.523	2229	488	0.014
6	14.835	3323	684	0.021
7	14.961	5532	1080	0.035
8	15.100	7448	1155	0.047
9	15.461	51451	5580	0.325
10	15.826	15570722	2372135	98.443
11	16.213	1073	243	0.007
12	16.389	17514	2812	0.111
13	16.555	113870	20369	0.720
14	16.796	6640	810	0.042
15	17.013	2902	525	0.018
16	17.276	2990	365	0.019
17	18.269	1060	233	0.007
18	21.192	2075	202	0.013
Total		15816931	2409017	100.000