

Sample Name :Gly-Arg-Gly-Asp-Asn-Pro
 Cat No. :RP10847
 Lot No. :PE2101904
 Time Processed :8:44:15
 Month-Day-Year Processed :05/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	75
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	15
40.00	Pumps	Solvent B Conc.	15
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

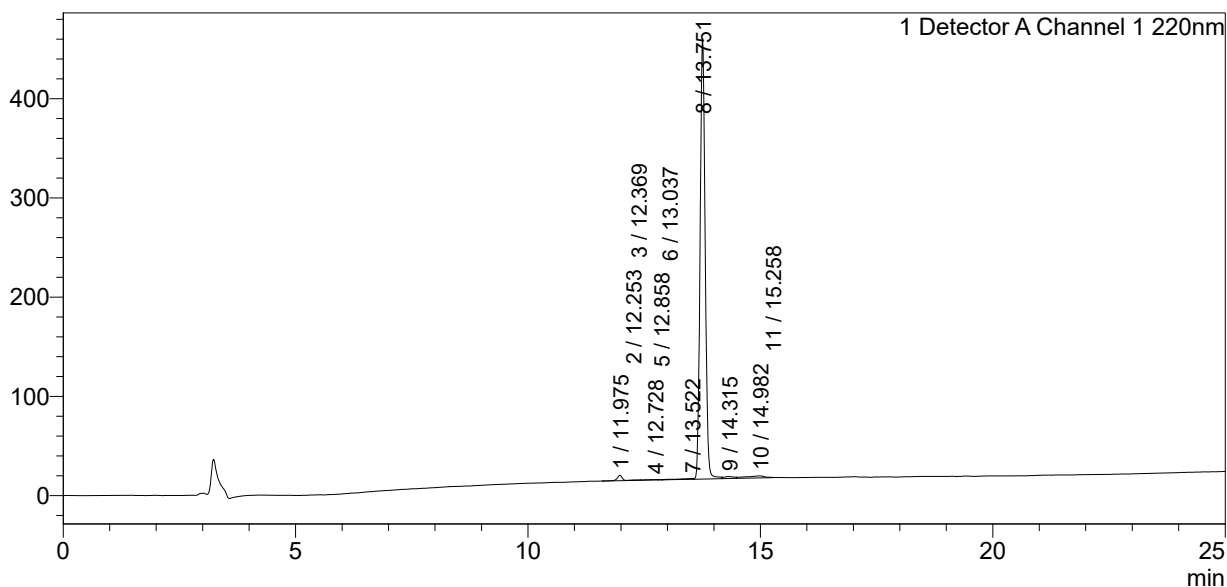

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.975	41915	5472	1.190
2	12.253	4661	499	0.132
3	12.369	2965	460	0.084
4	12.728	9468	486	0.269
5	12.858	1634	340	0.046
6	13.037	5596	470	0.159
7	13.522	15960	842	0.453
8	13.751	3353043	443862	95.168
9	14.315	29743	2004	0.844
10	14.982	57714	1997	1.638
11	15.258	599	137	0.017
Total		3523298	456570	100.000