


Mass Spectrum

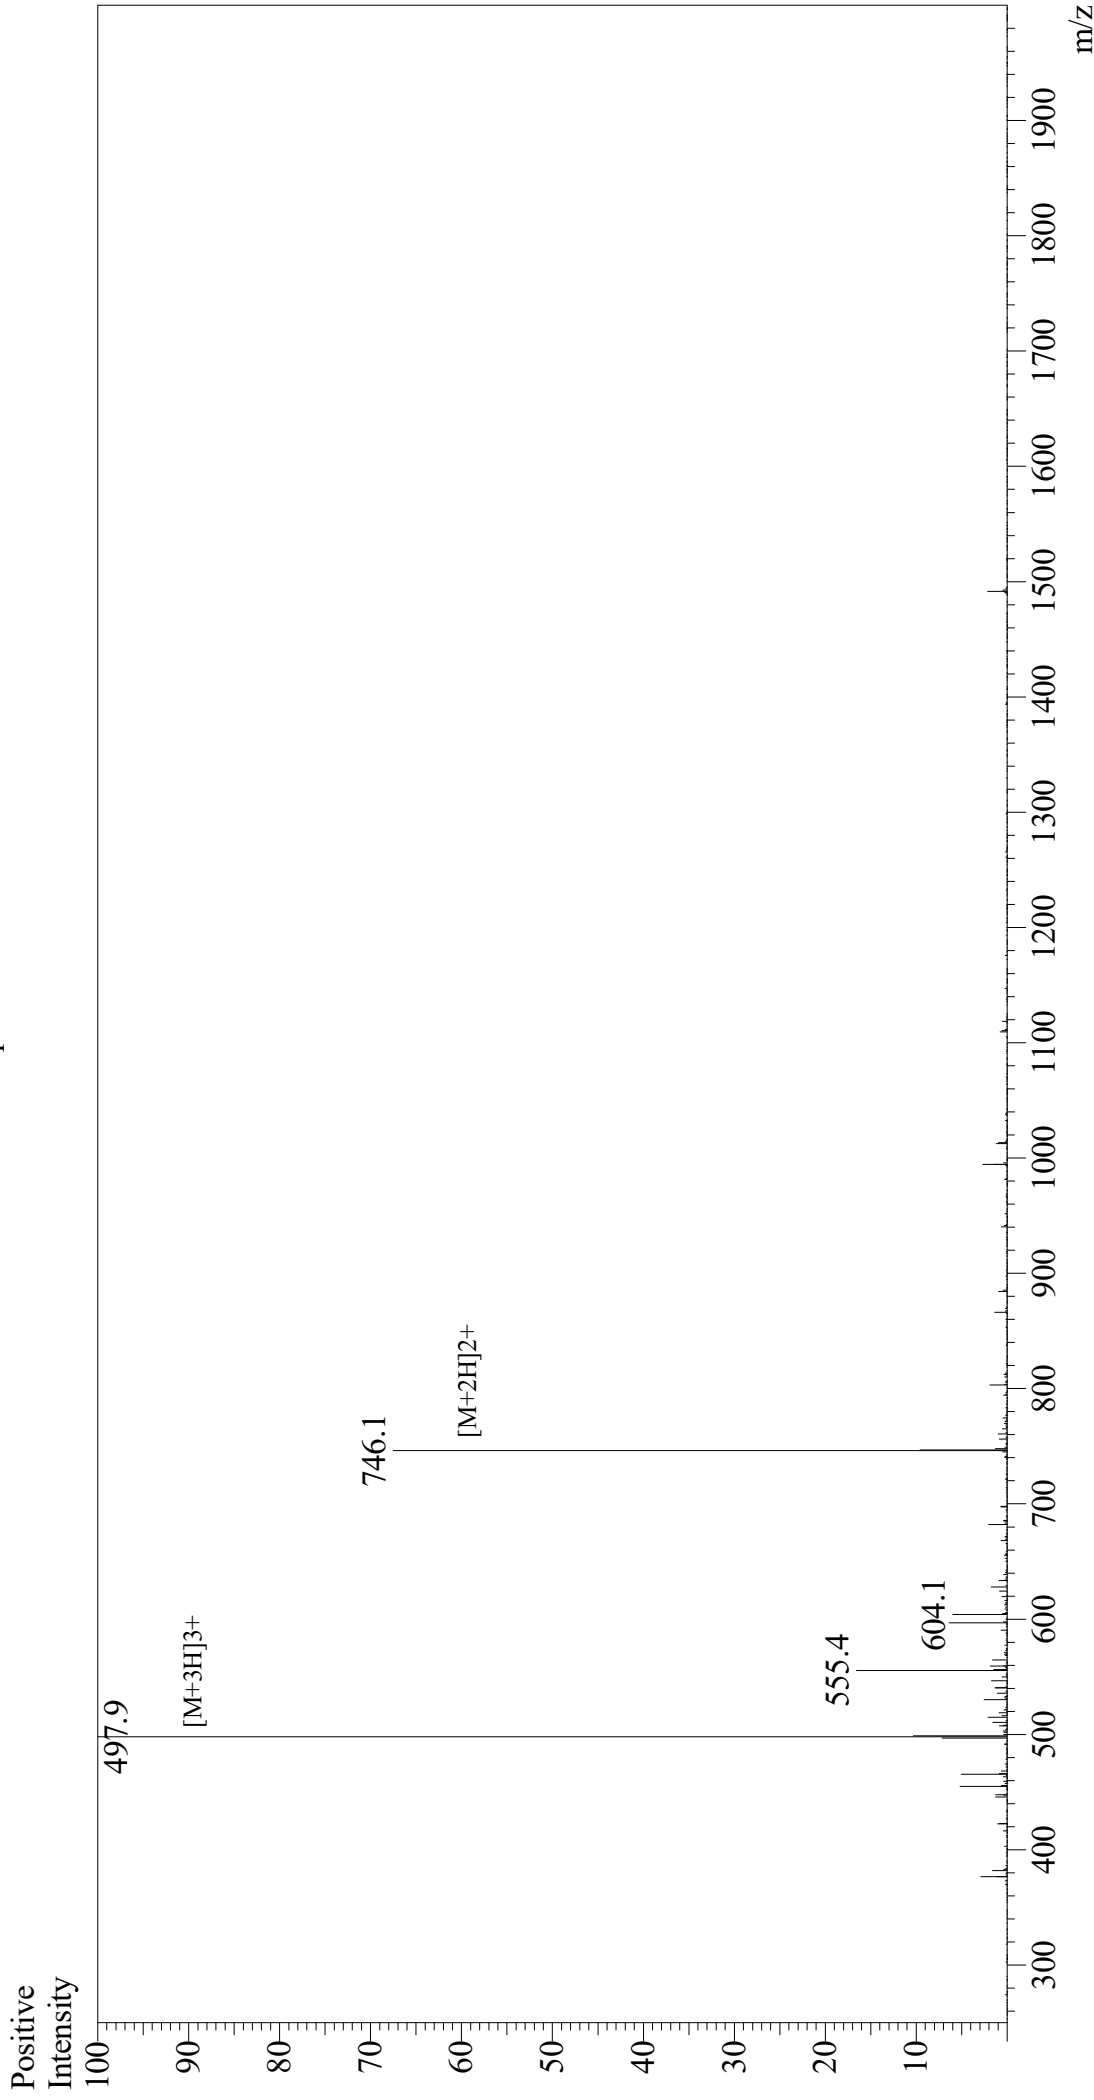

Sample Information

Month-Day Processed : 05/08/21
Time Processed : 9:13:41 AM
Injection Volume : 0.4
Sample Name : SV40 T-Ag-derived NLS peptide
Cat No. : RP20513
Lot No. : E2670821E
Theoretical MW : 1490.80
Observed MW : 1490.7

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH