

Sample Name :Angiotensin I, human
 Cat No. : RP11251
 Lot No. : PE8421902
 Time Processed : 7:03:45
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

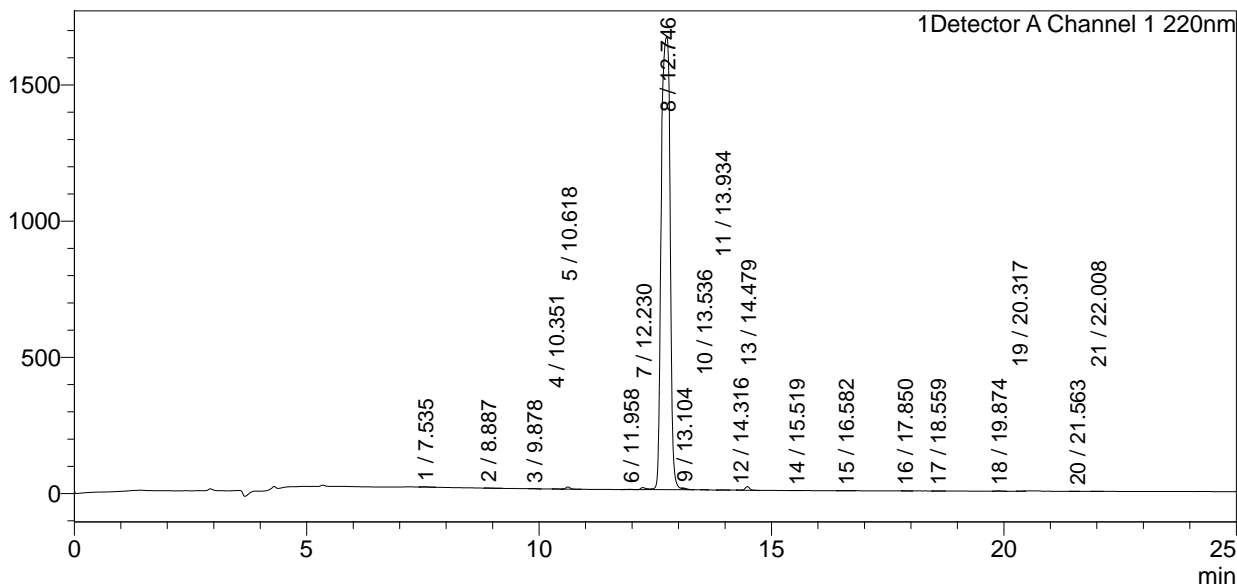

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.535	9946	1488	0.045
2	8.887	4957	616	0.022
3	9.878	8591	1265	0.039
4	10.351	3972	662	0.018
5	10.618	52487	8254	0.236
6	11.958	8210	998	0.037
7	12.230	68627	7496	0.308
8	12.746	21983641	1663816	98.714
9	13.104	8071	1792	0.036
10	13.536	1782	420	0.008
11	13.934	4633	658	0.021
12	14.316	1528	344	0.007
13	14.479	89343	13786	0.401
14	15.519	1295	189	0.006
15	16.582	5174	437	0.023

Peak#	Ret. Time	Area	Height	Area%
16	17.850	1535	188	0.007
17	18.559	2146	224	0.010
18	19.874	8924	1262	0.040
19	20.317	1023	144	0.005
20	21.563	1839	203	0.008
21	22.008	2397	331	0.011
Total		22270122	1704573	100.000