

Sample Name : β -Amyloid (1-42), rat
 Cat. No. : RP10013
 Lot. No. : E9472120B
 Time Processed : 14:44:58
 Month-Day-Year Processed : 03/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

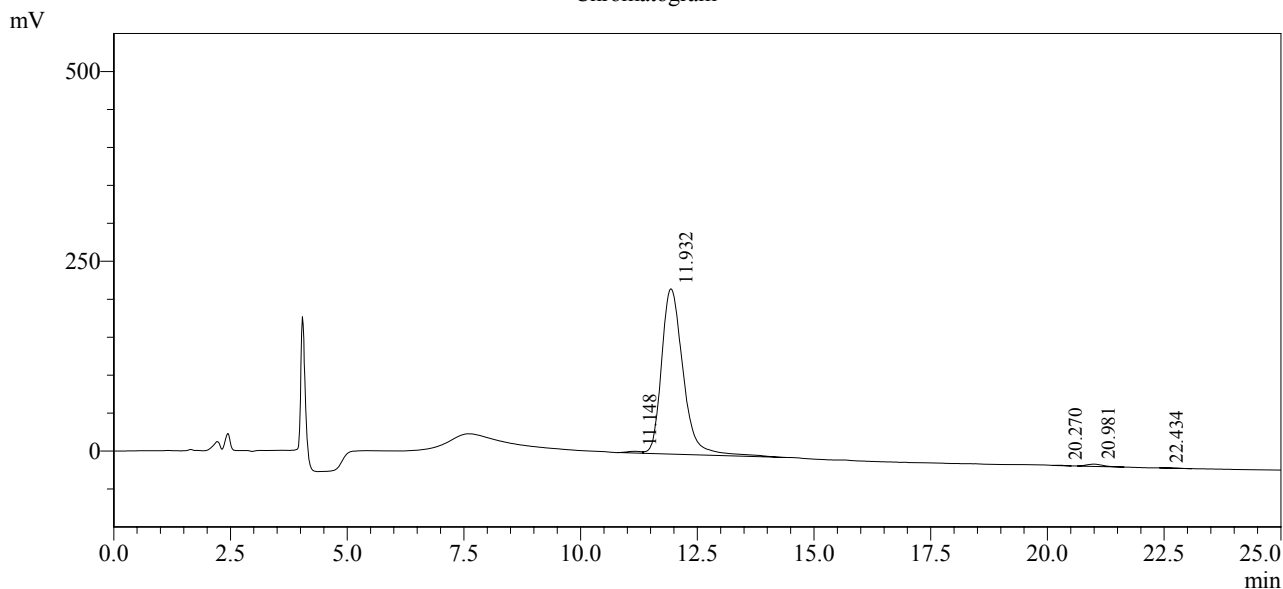

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.148	46843	2246	0.655
2	11.932	7023611	217855	98.150
3	20.270	4939	458	0.069
4	20.981	71203	2920	0.995
5	22.434	9412	226	0.132
Total		7156009	223705	100.000