

Sample Name : -Factor Mating Pheromone, yeast
 Cat No :RP01002
 Lot No :E5234321D
 Time Processed :1:51:20 AM
 Month-Day-Year Processed :04/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

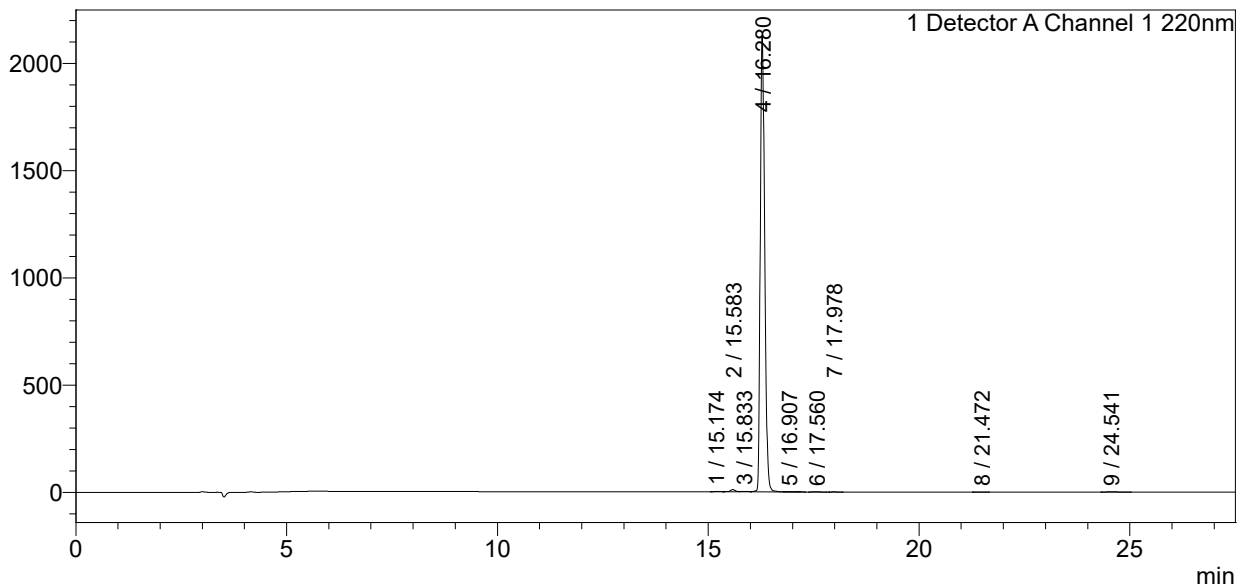

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.174	22569	1913	0.143
2	15.583	96503	10752	0.611
3	15.833	33701	2674	0.213
4	16.280	15593966	2124869	98.766
5	16.907	4519	553	0.029
6	17.560	6207	884	0.039
7	17.978	2155	300	0.014
8	21.472	4553	450	0.029
9	24.541	24685	1423	0.156
Total		15788858	2143817	100.000