

Sample Name : -Amyloid (1-42), rat
 Cat. No. : RP10013
 Lot. No. : E2692521A
 Time Processed :1:58:59 PM
 Month-Day-Year Processed :01/08/2021
 Pump A : 0.5% ammonia water in 100% water (v/v)
 Pump B : 0.2% ammonia water in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil UniPS 4.6 x 250 mm
 Equipment: GR11010440

<Chromatogram>

mV

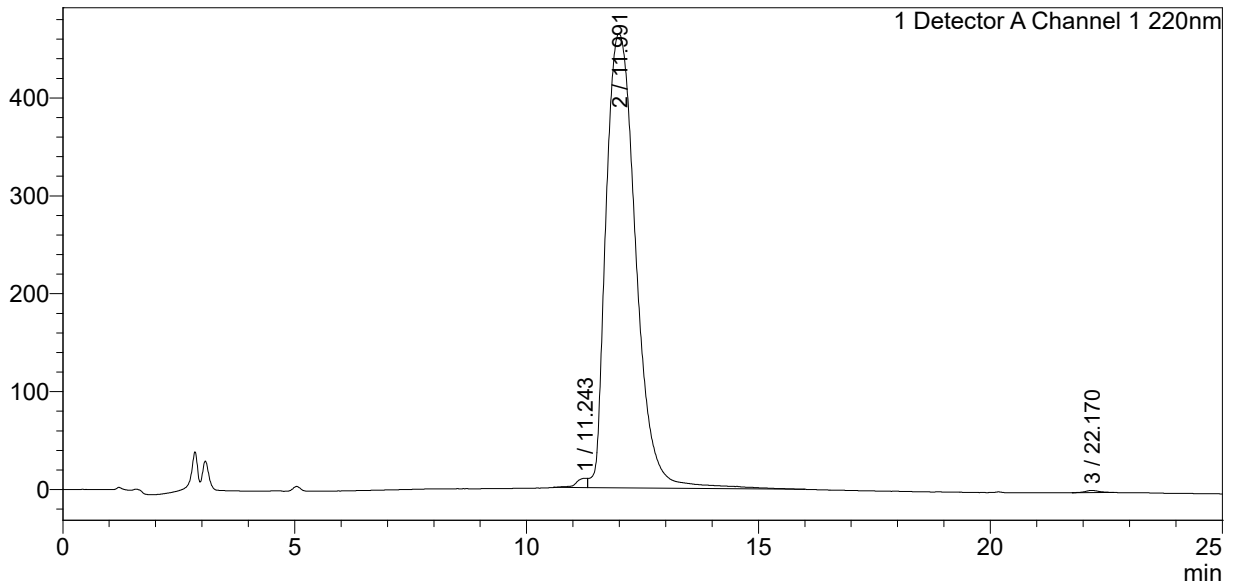

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.243	162276	9527	0.775
2	11.991	20741820	464073	99.014
3	22.170	44211	2208	0.211
Total		20948307	475808	100.000