

Sample Name :GRGDSPC
 Cat. No. : RP20283
 Lot. No. :PE8551905
 Time Processed :17:59:31
 Month-Day-Year Processed :06/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

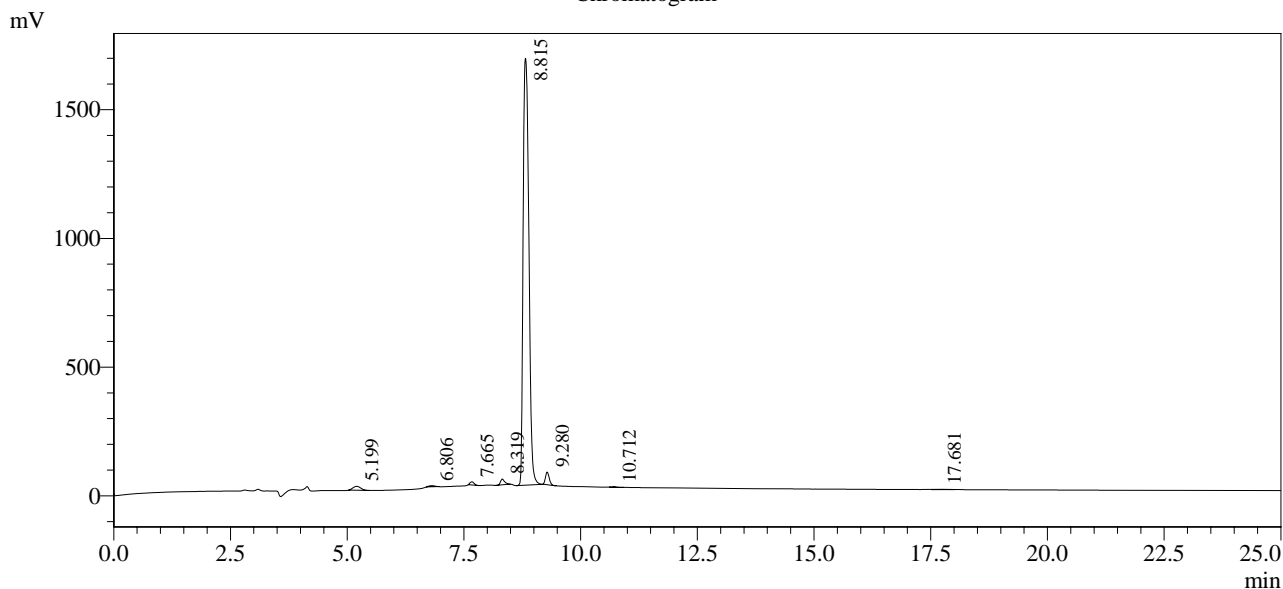

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.199	180120	15429	1.211
2	6.806	37399	4103	0.251
3	7.665	71826	12258	0.483
4	8.319	137819	22552	0.926
5	8.815	14149013	1658887	95.095
6	9.280	275885	49503	1.854
7	10.712	10976	2135	0.074
8	17.681	15728	1596	0.106
Total		14878767	1766462	100.000