

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), rat
 Cat. No. :RP11195
 Lot. No. :E3976420I
 Time Processed : 2:51:38 PM
 Month-Day-Year Processed : 10/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

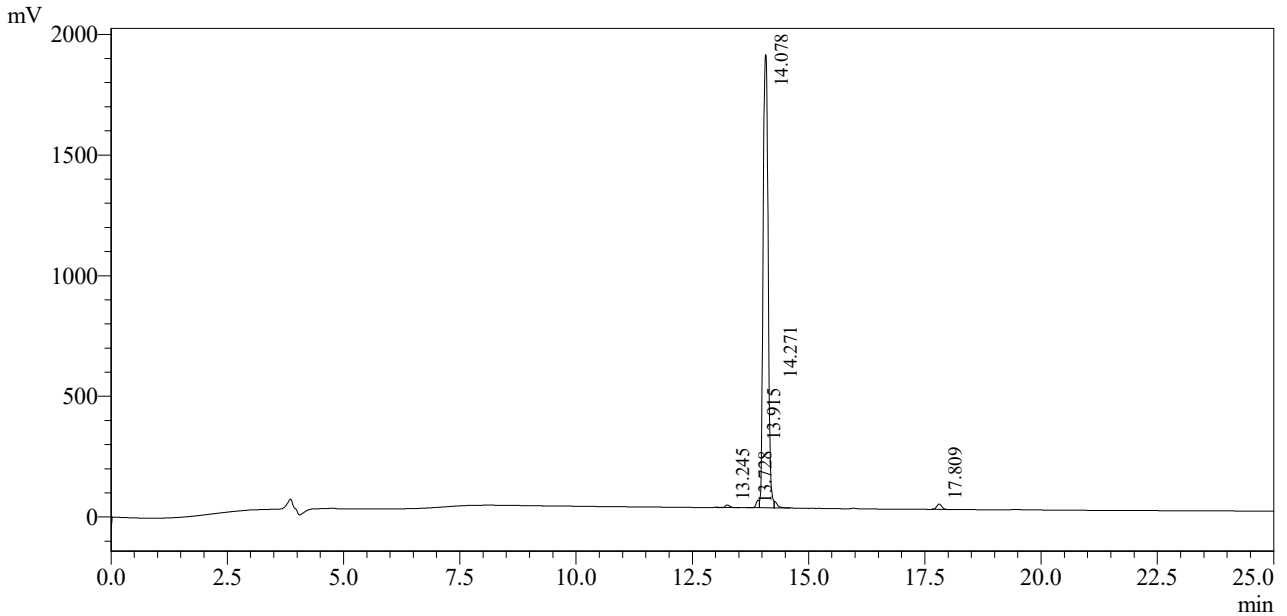

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.245	63802	10957	0.439
2	13.728	2503	659	0.017
3	13.915	140107	31406	0.965
4	14.078	14031614	1877359	96.603
5	14.271	119836	26906	0.825
6	17.809	167230	21740	1.151
Total		14525093	1969026	100.000