


Mass Spectrum

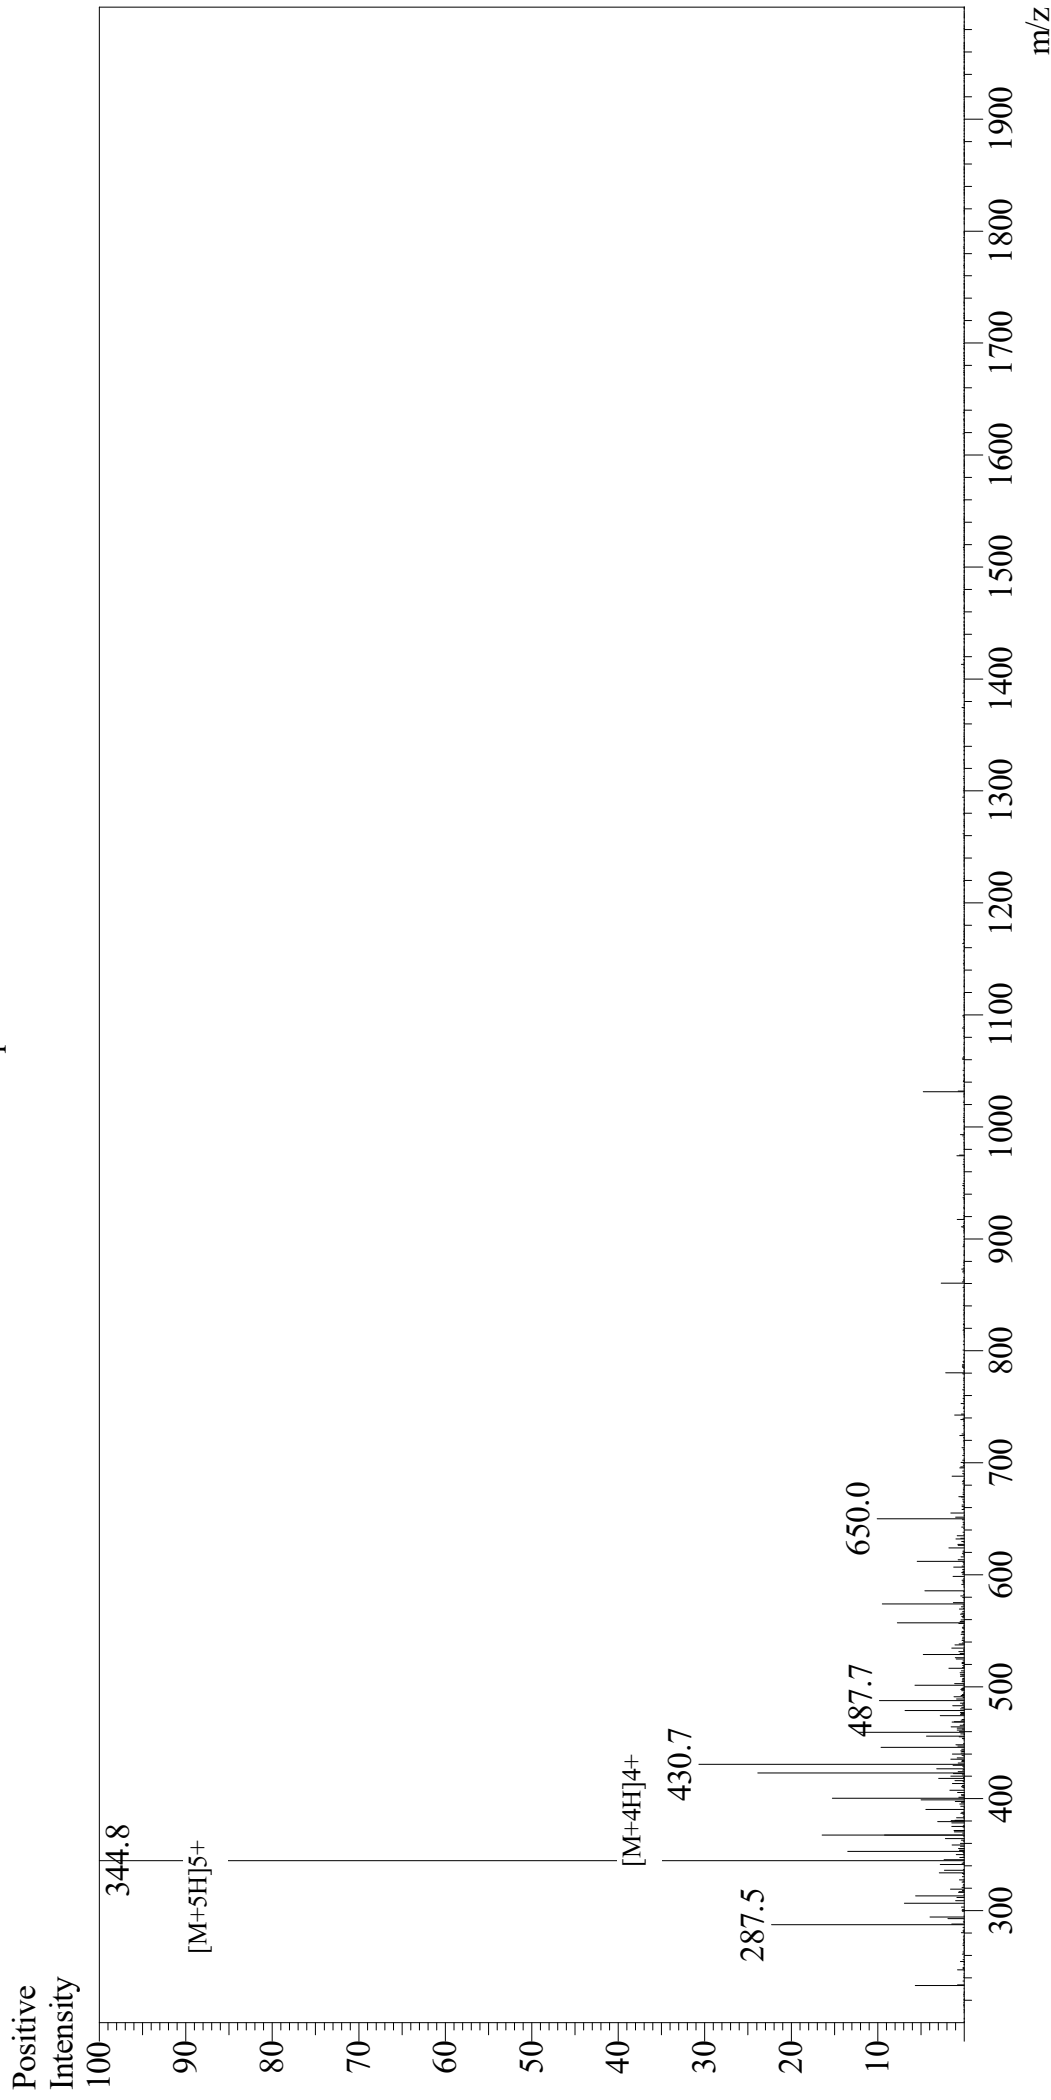

Sample Information
User : Gary
Month-Day Processed : 09/19/19
Time Processed : 08:58:44 PM
Injection Volume : 0.4
Sample Name : HIV-1 TAT (48-60)
Cat No. : RP20423
Lot No. : E496519I
Theoretical MW : 1719.00
Observed MW : 1719.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH