

Sample Name : [Glu1]-Fibrinopeptide B  
 Cat. No. :RP20439  
 Lot. No. :E4962519I  
 Time Processed :14:18:26  
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

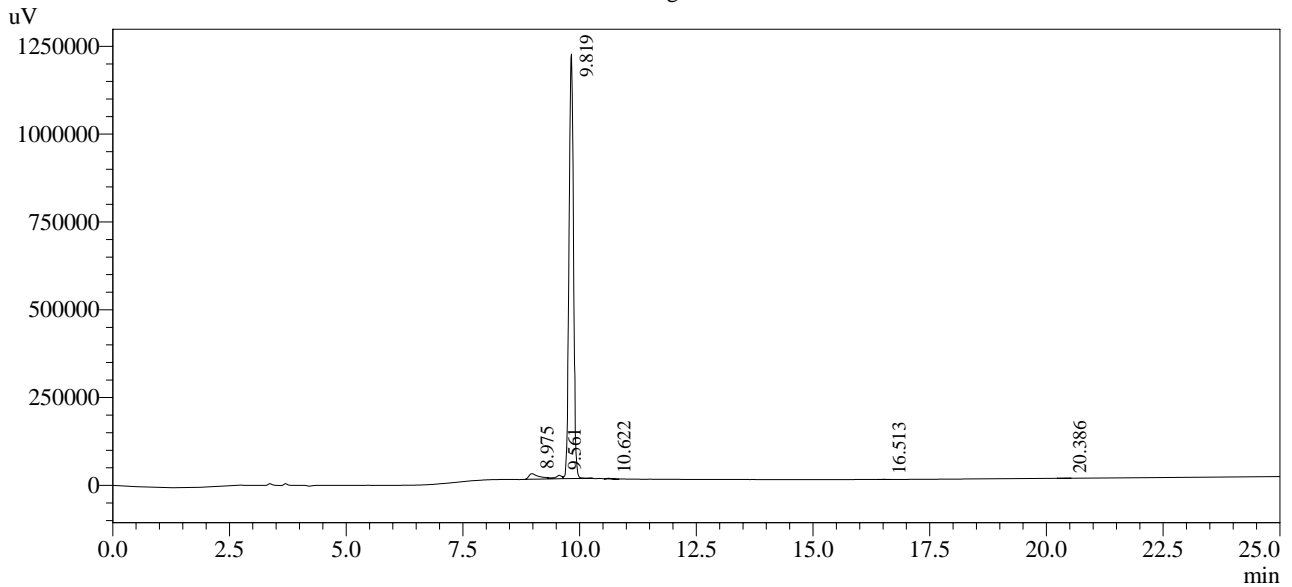

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.975	230724	15463	2.748
2	9.561	98992	9588	1.179
3	9.819	8050684	1203337	95.889
4	10.622	9834	1876	0.117
5	16.513	2101	363	0.025
6	20.386	3492	528	0.042
Total		8395828	1231155	100.000