

Sample Name :HIV p17 Gag (77-85)
 Cat No. :RP17316
 Lot No. :E1396721G
 Time Processed :21:39:46
 Month-Day-Year Processed :07/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

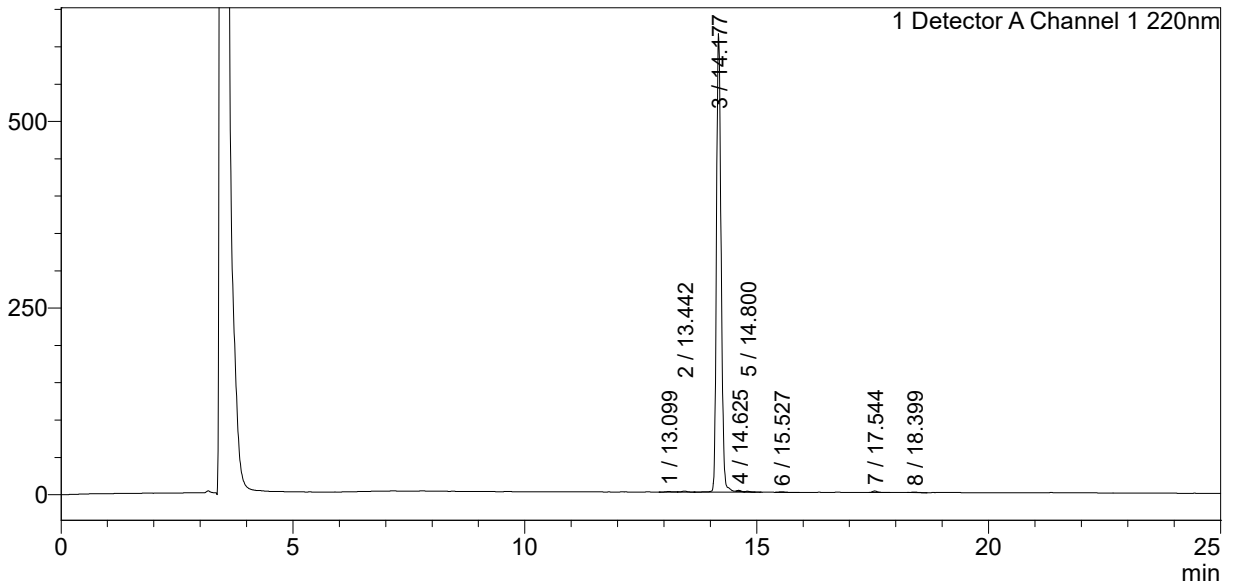

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.099	7846	697	0.179
2	13.442	11856	1492	0.271
3	14.177	4318416	592623	98.644
4	14.625	6540	1378	0.149
5	14.800	4671	864	0.107
6	15.527	8050	880	0.184
7	17.544	15180	1993	0.347
8	18.399	5224	643	0.119
Total		4377782	600570	100.000