

Sample Name : c-Myc Peptide  
 Cat. No. : RP11731  
 Lot. No. : E6344221A

Time Processed: 15:55:29  
 Year-Month-Day: 2021/2/8

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

<<Detector A>>

Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010015

<Chromatogram>

mV

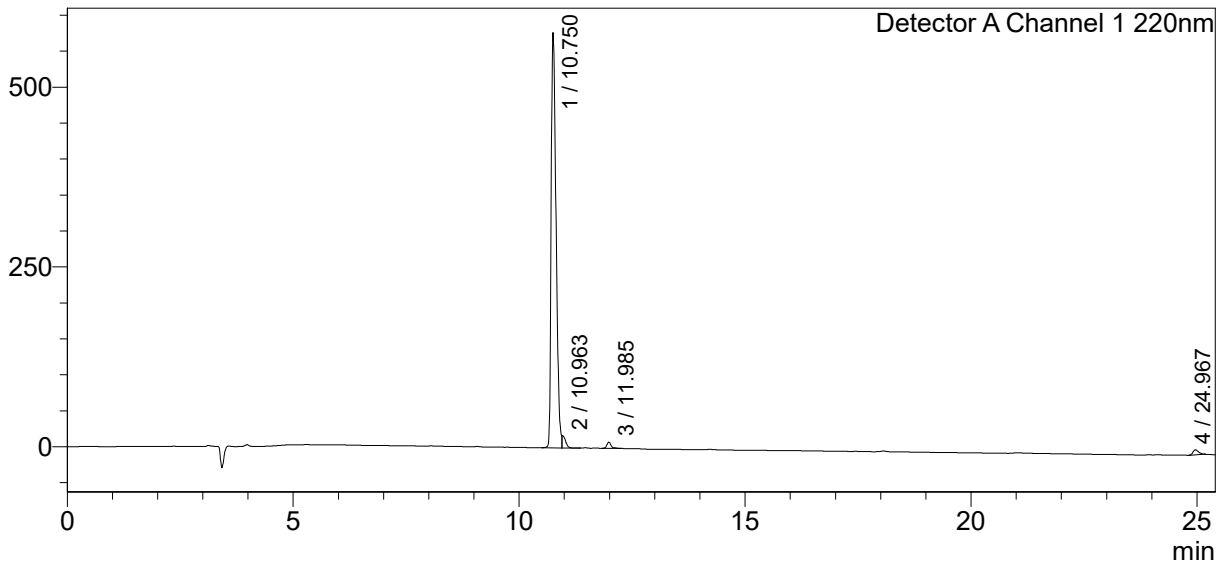

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.750	4336022	577530	95.465
2	10.963	87682	16980	1.930
3	11.985	57397	8807	1.264
4	24.967	60881	6974	1.340
Total		4541983	610291	100.000