


Mass Spectrum

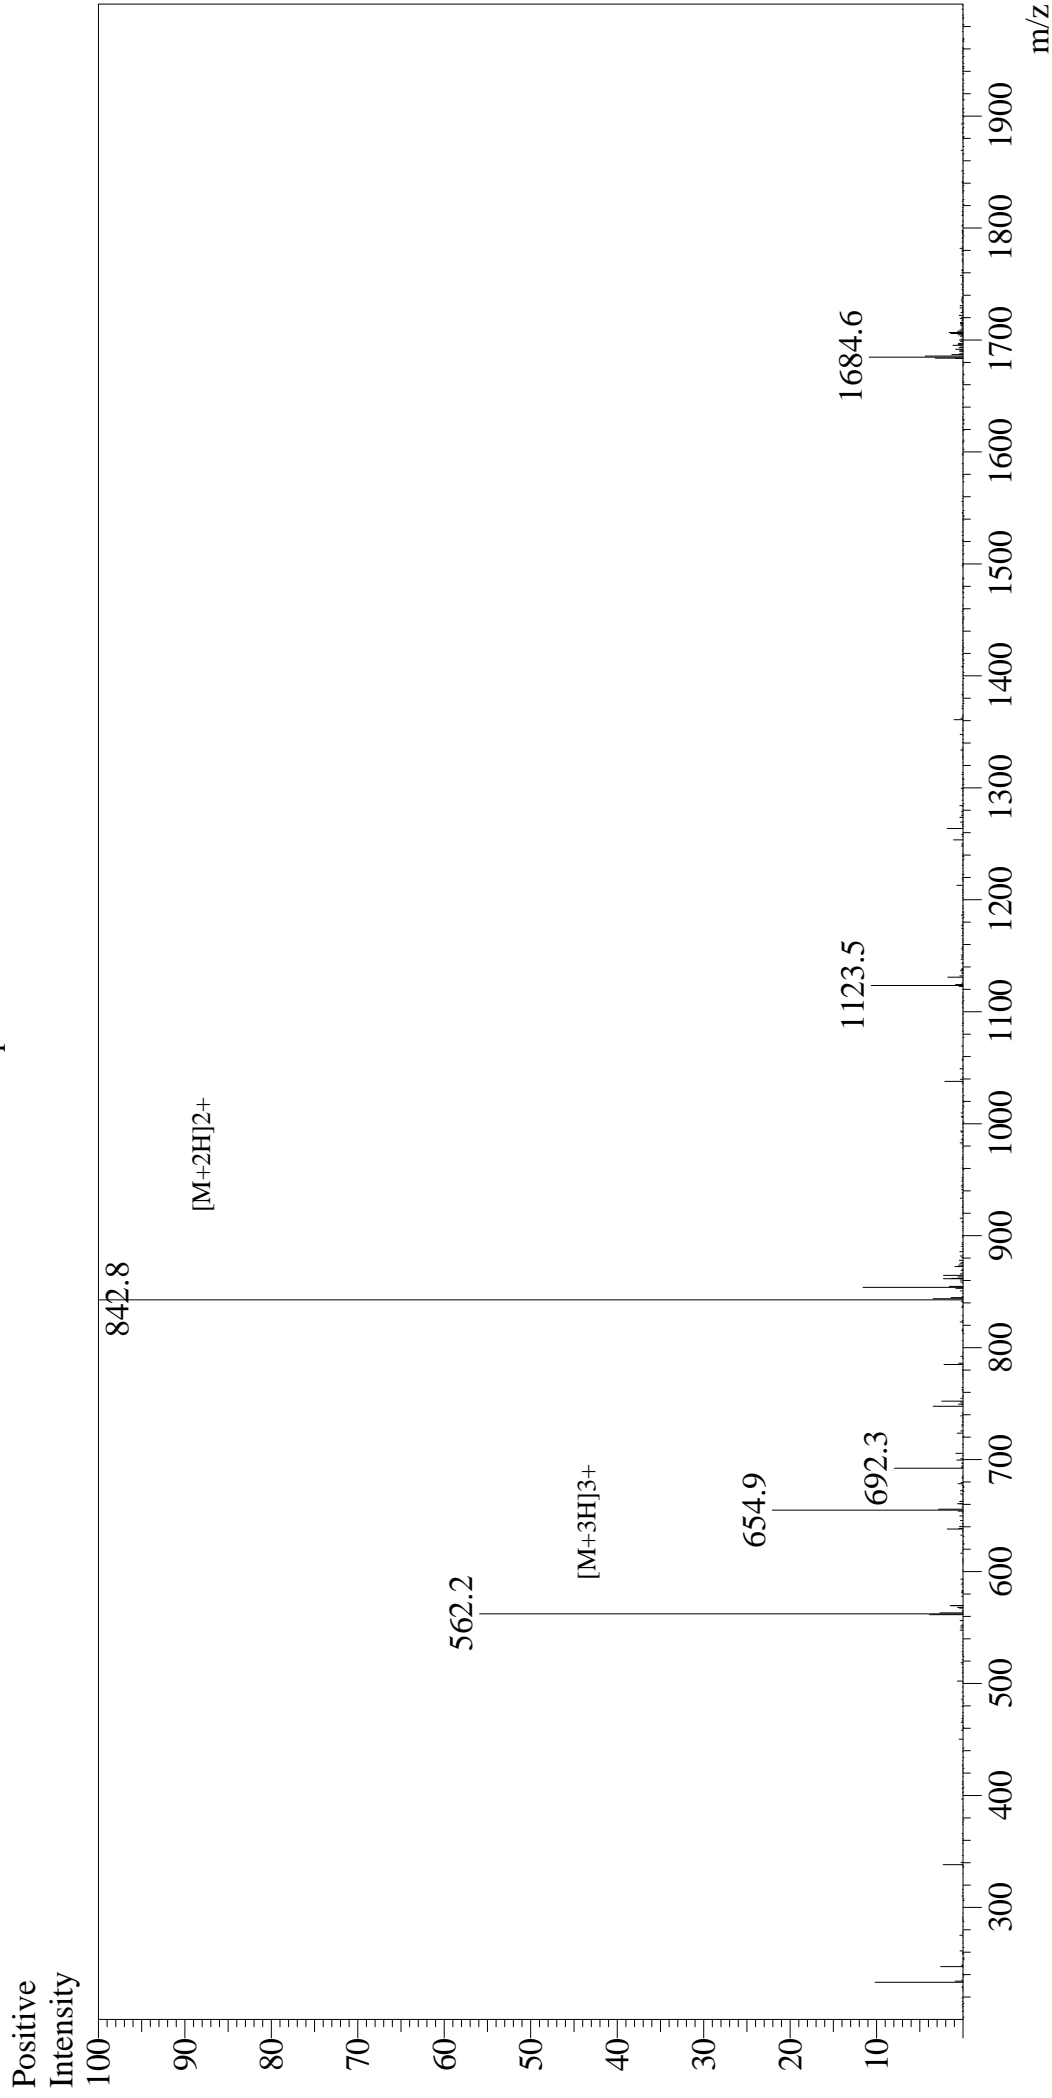

Sample Information

User : Gary
 Month-Day Processed : 09/09/19
 Time Processed : 16:22:14
 Injection Volume : 0.3
 Sample Name : α -Factor Mating Pheromone, yeast
 Cat No. : RP01002
 Lot No. : E9582319H
 Theoretical MW : 1683.98
 Observed MW : 1683.6

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2ml/min
 B.conc : 50%H₂O/50%MeOH