

Sample Name : β -Amyloid (35-25)
 Cat No. :RP20185
 Lot No. :E4830019I
 Time Processed :9:55:44 AM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

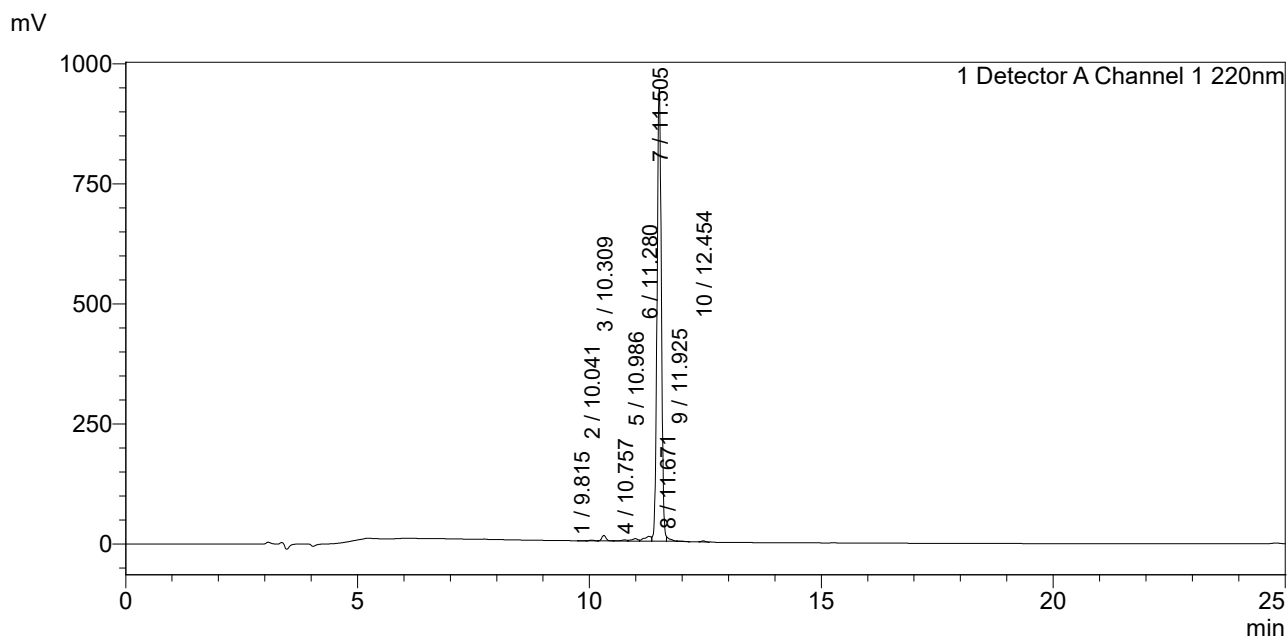

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.815	1059	206	0.016
2	10.041	12893	1894	0.200
3	10.309	73855	11580	1.144
4	10.757	21516	2457	0.333
5	10.986	47497	5107	0.736
6	11.280	104738	9918	1.623
7	11.505	6132153	943213	95.001
8	11.671	46559	9249	0.721
9	11.925	3164	212	0.049
10	12.454	11429	2151	0.177
Total		6454863	985987	100.000