

Sample Name :N-Boc-Phe-Leu-Phe-Leu-Phe
 Cat No. :RP12950
 Lot No. :E8007920I
 Time Processed : 22:34:36
 Month-Day-Year Processed : 09/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
37.00	Pumps	Pump B Conc.	95
37.01	Pumps	Pump B Conc.	5
42.00	Pumps	Pump B Conc.	5
42.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

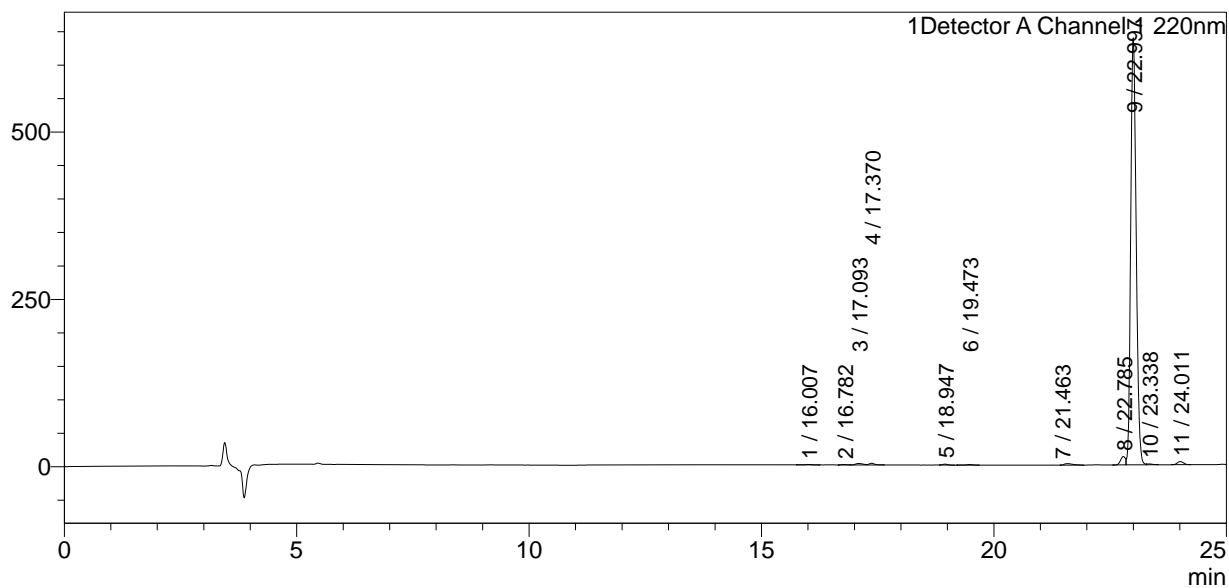

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.007	5937	682	0.109
2	16.782	4268	565	0.078
3	17.093	23530	2067	0.432
4	17.370	19334	2451	0.355
5	18.947	9243	1326	0.170
6	19.473	8626	829	0.159
7	21.463	27633	169	0.508
8	22.785	90599	12475	1.665
9	22.997	5198956	638006	95.548
10	23.338	9918	1271	0.182
11	24.011	43181	4588	0.794
Total		5441225	664428	100.000