

Sample Name : Melanotan (MT)-II
 Cat. No. : RP17323
 Lot. No. : PE3351612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

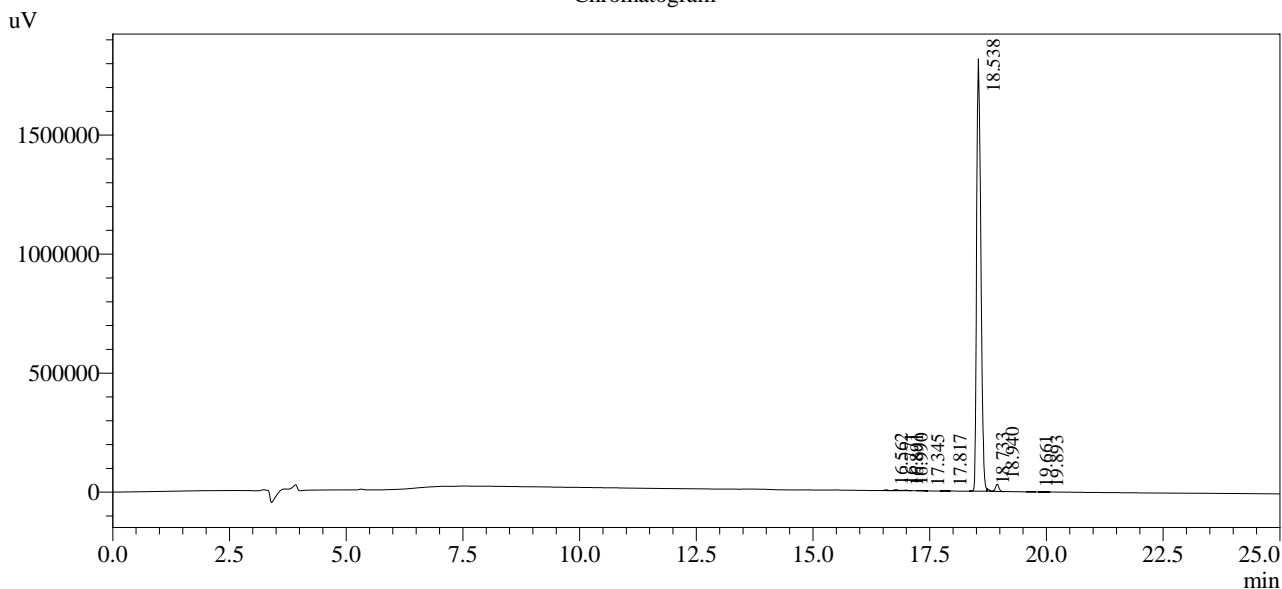

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.562	18257	3443	0.155
2	16.771	27057	4246	0.230
3	16.891	6444	1590	0.055
4	16.990	12579	2534	0.107
5	17.345	6993	1018	0.059
6	17.817	6548	1275	0.056
7	18.538	11496170	1816440	97.760
8	18.733	29494	9997	0.251
9	18.940	151823	30414	1.291
10	19.661	2413	497	0.021
11	19.893	1795	261	0.015
Total		11759573	1871717	100.000