

Sample Name :GRGDSPC
 Cat. No. : RP20283
 Lot. No. : E7770219F
 Time Processed : 10:25:02
 Month-Day-Year Processed : 06/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
31.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

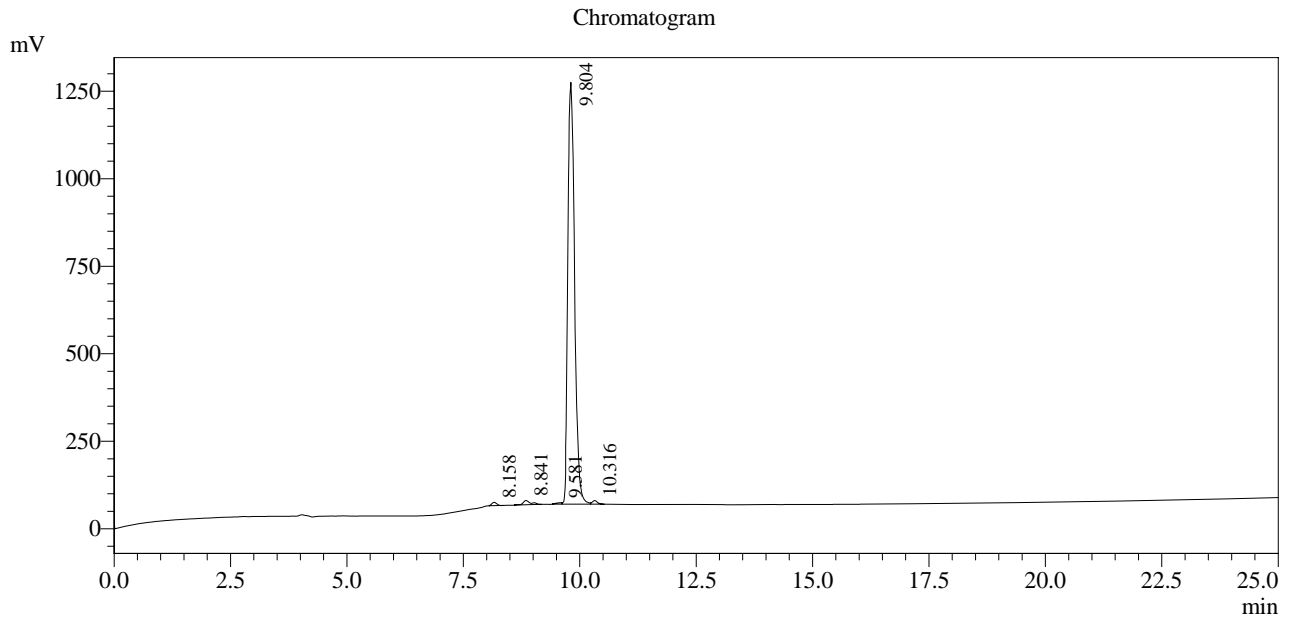

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.158	66696	9360	0.533
2	8.841	143373	12281	1.146
3	9.581	36789	4270	0.294
4	9.804	12186275	1204618	97.419
5	10.316	75939	10162	0.607
Total		12509073	1240692	100.000