

Sample Name : Physalaemin  
 Cat. No. : RP10474  
 Lot. No. : E9407320B  
 Time Processed :9:19:01  
 Month-Day-Year Processed :02/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

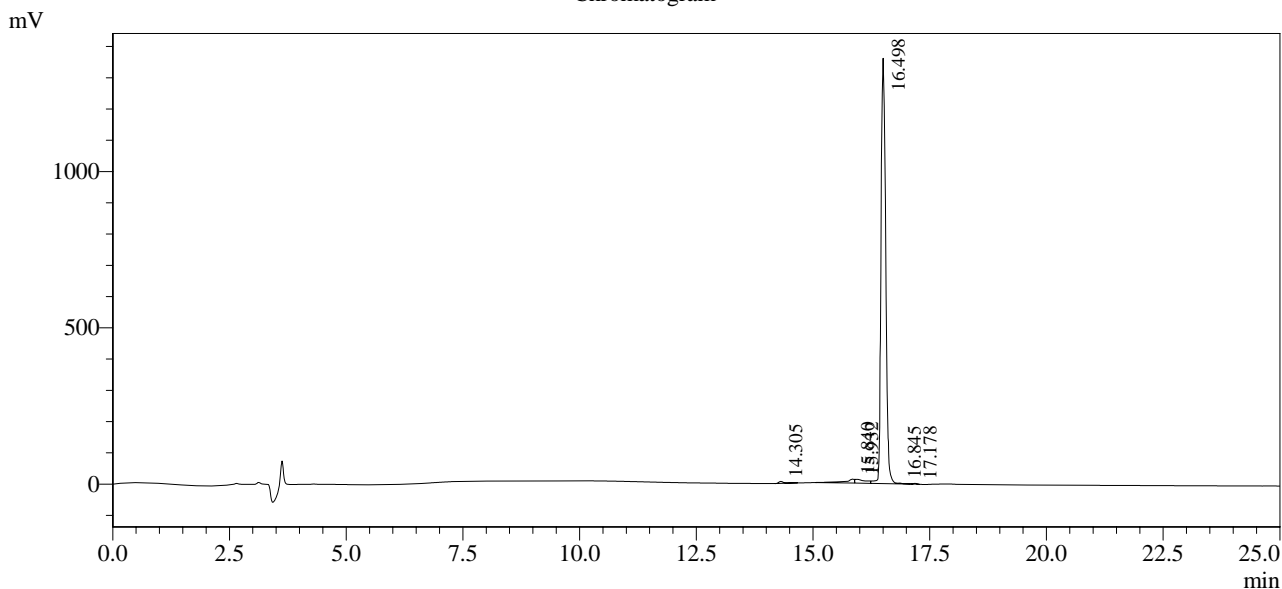

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.305	51326	6356	0.514
2	15.840	192840	12347	1.931
3	15.932	191127	12307	1.914
4	16.498	9524220	1360816	95.364
5	16.845	16616	2434	0.166
6	17.178	11138	2453	0.112
Total		9987267	1396712	100.000