


Mass Spectrum

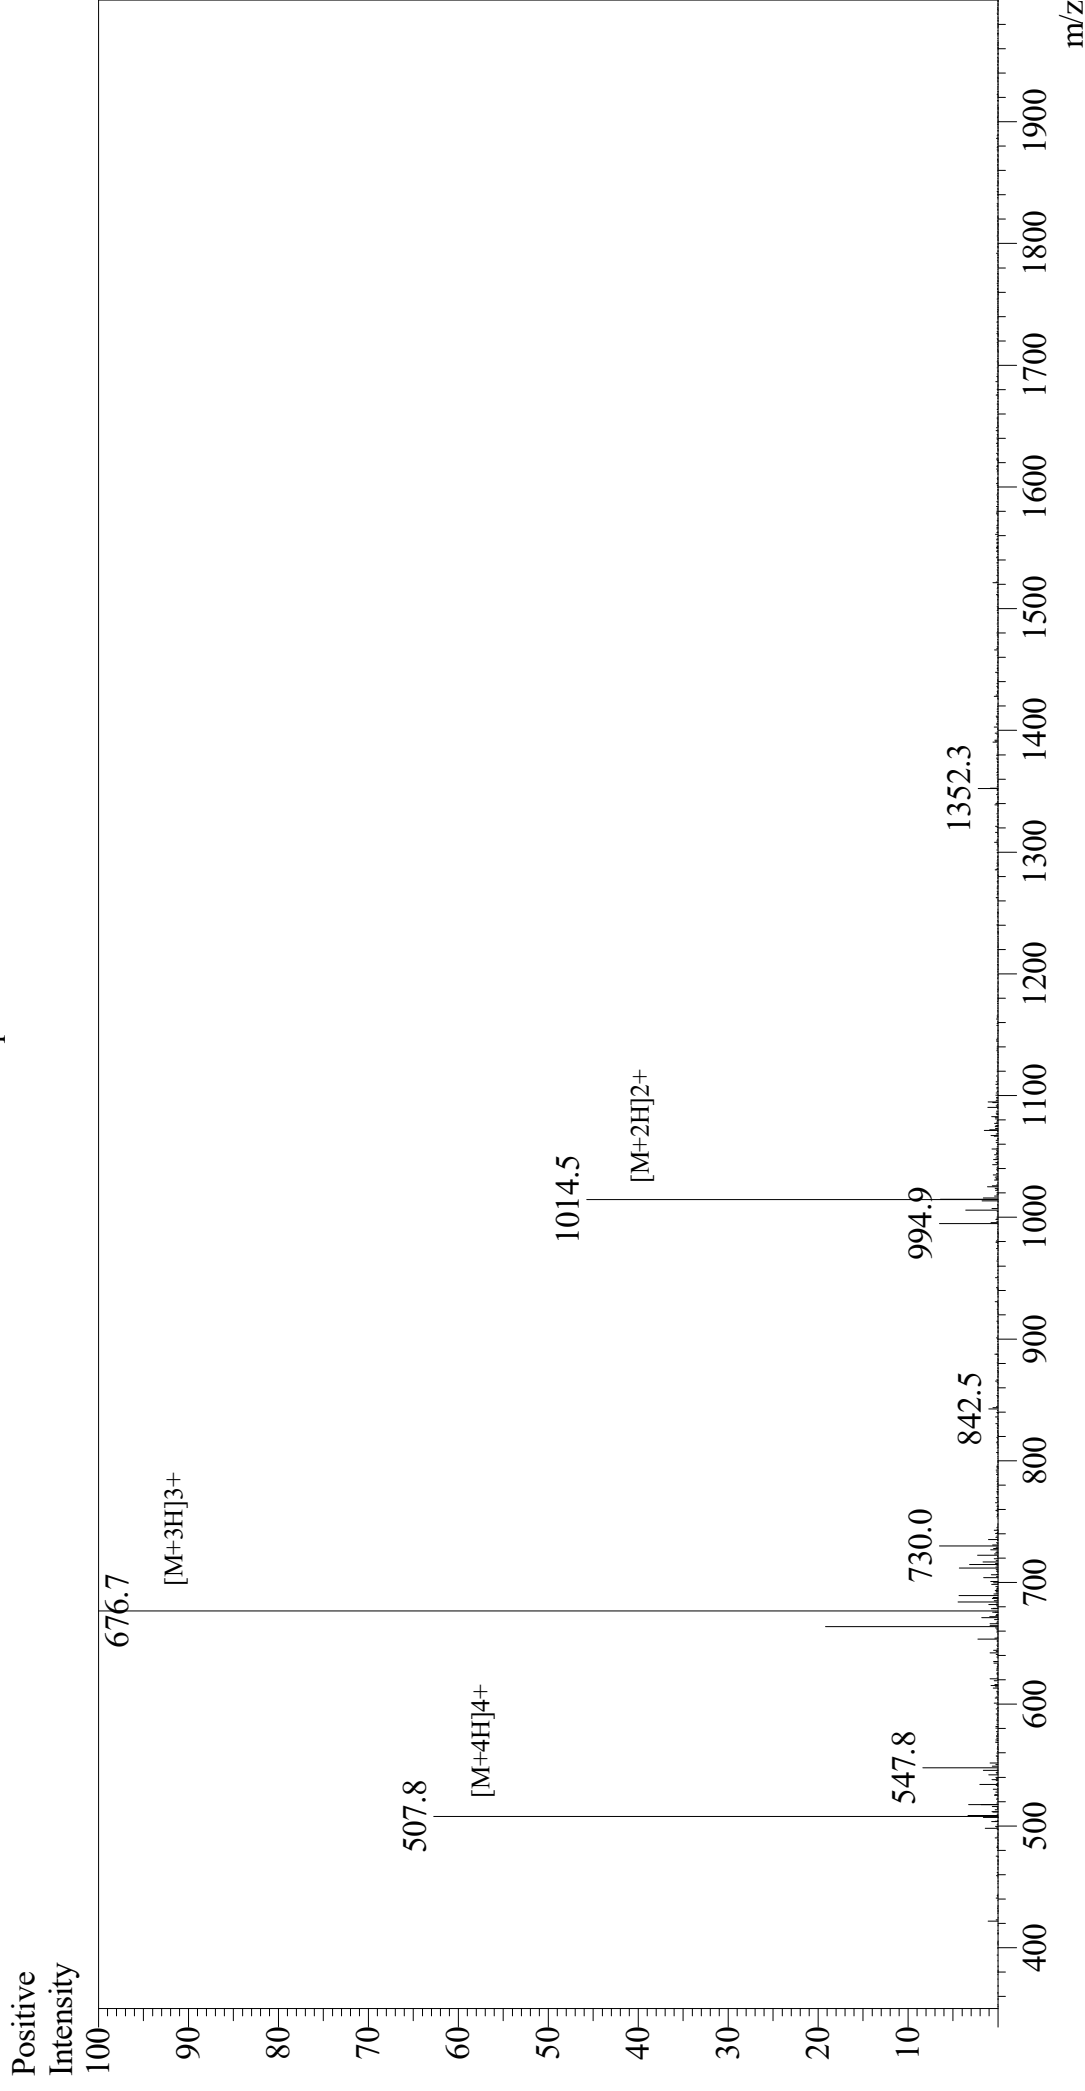

Sample Information

Month-Day Processed : 12/19/21
Time Processed : 21:44:10
Injection Volume : 0.4
Sample Name : Apamin
Cat No. : RP11002
Lot No. : E6159321L
Theoretical MW : 2027.30
Observed MW : 2027.1

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH