


Mass Spectrum

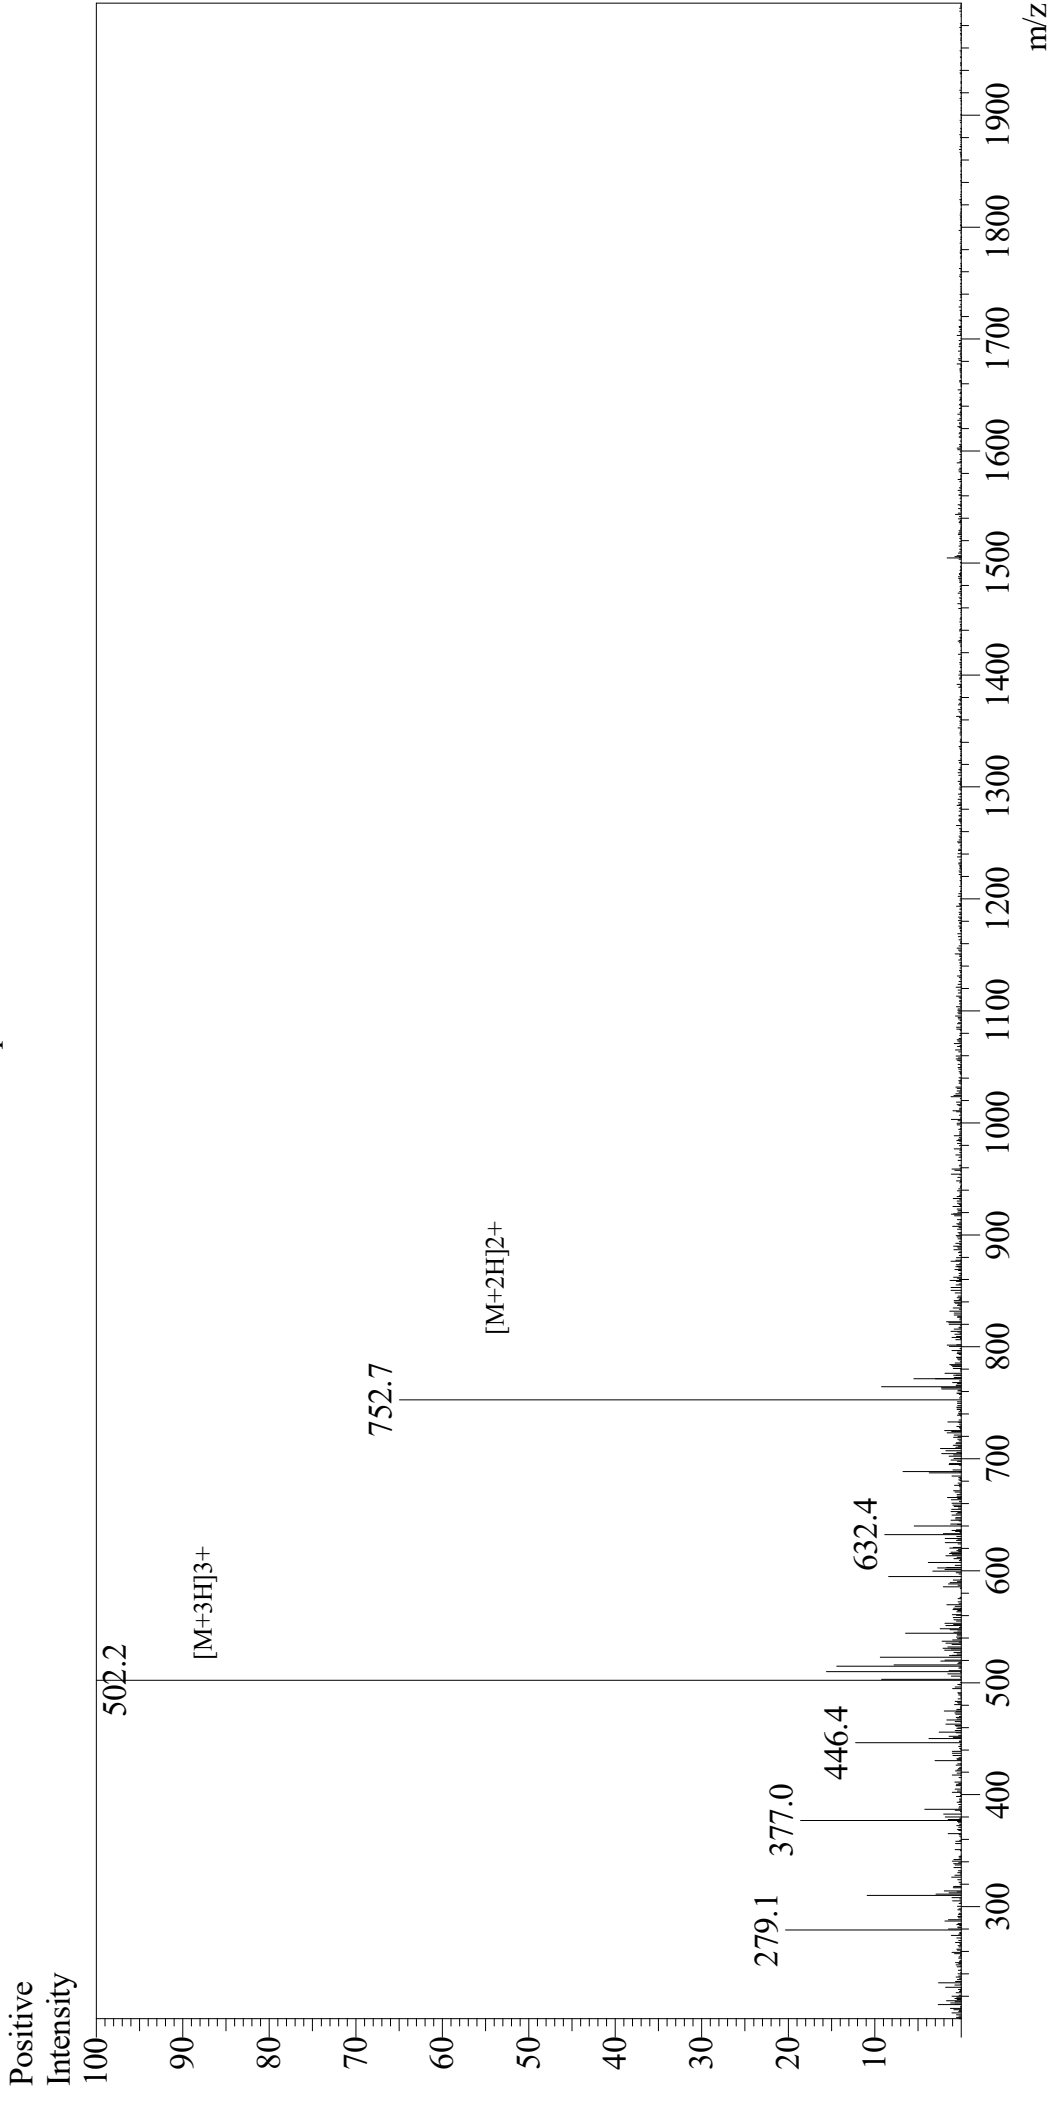

Sample Information		Equipment	
Month-Day Processed :	09/26/20	Interface	:GK11010007
Time Processed :	07:29:30 AM	Nebulizing Gas Flow	:+4.5kV
Injection Volume :	0.3	CDL Temp	:5 L/min
Sample Name :	Influenza Hemagglutinin (307-319)	Drying Gas Flow	:0.2ml/min
Cat No. :	RP20087	Block Temp	:50%H2O/50%MeOH
Lot No. :	E8001520I		
Theoretical MW :	1503.79		
Observed MW :	1804.5		