

Sample Name : $\delta$ -Sleep Inducing Peptide  
 Cat No. :RP10580  
 Lot No. :E6999619J  
 Time Processed :7:22:09  
 Month-Day-Year Processed :10/02/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

<Chromatogram>

mV

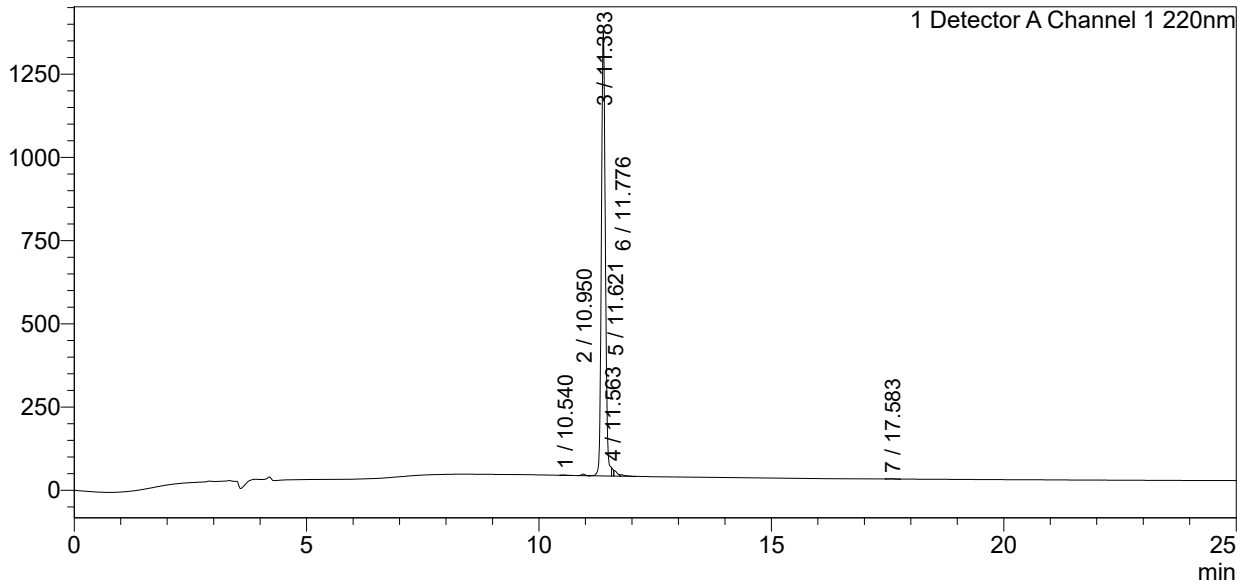

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.540	5269	952	0.065
2	10.950	23657	4545	0.291
3	11.383	7926812	1332288	97.438
4	11.563	61618	25778	0.757
5	11.621	79656	17028	0.979
6	11.776	31842	4262	0.391
7	17.583	6372	1028	0.078
Total		8135226	1385881	100.000