

Sample Name :BDC2.5 mimotope 1040-31
 Cat. No. :RP20518
 Lot. No. E45574219J
 Time Processed : 7:15:54
 Month-Day-Year Processed :10/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

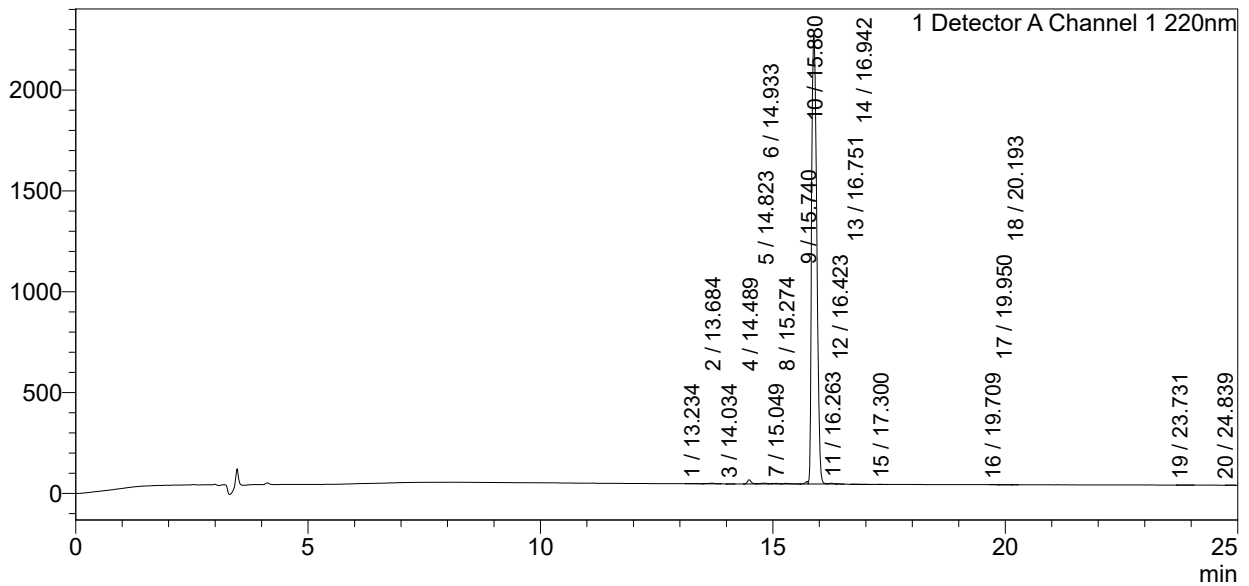

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.234	5043	483	0.029
2	13.684	29530	3253	0.169
3	14.034	1219	217	0.007
4	14.489	116128	20838	0.666
5	14.823	40116	4305	0.230
6	14.933	8883	2113	0.051
7	15.049	28371	3451	0.163
8	15.274	30989	3518	0.178
9	15.740	55526	12852	0.318
10	15.880	17072528	2228467	97.886
11	16.263	27012	4329	0.155
12	16.423	6743	1494	0.039
13	16.751	2820	548	0.016
14	16.942	1465	247	0.008
15	17.300	2560	398	0.015

Peak#	Ret. Time	Area	Height	Area%
16	19.709	2093	287	0.012
17	19.950	3055	281	0.018
18	20.193	1550	388	0.009
19	23.731	2899	219	0.017
20	24.839	2717	397	0.016
Total		17441247	2288083	100.000