


Mass Spectrum

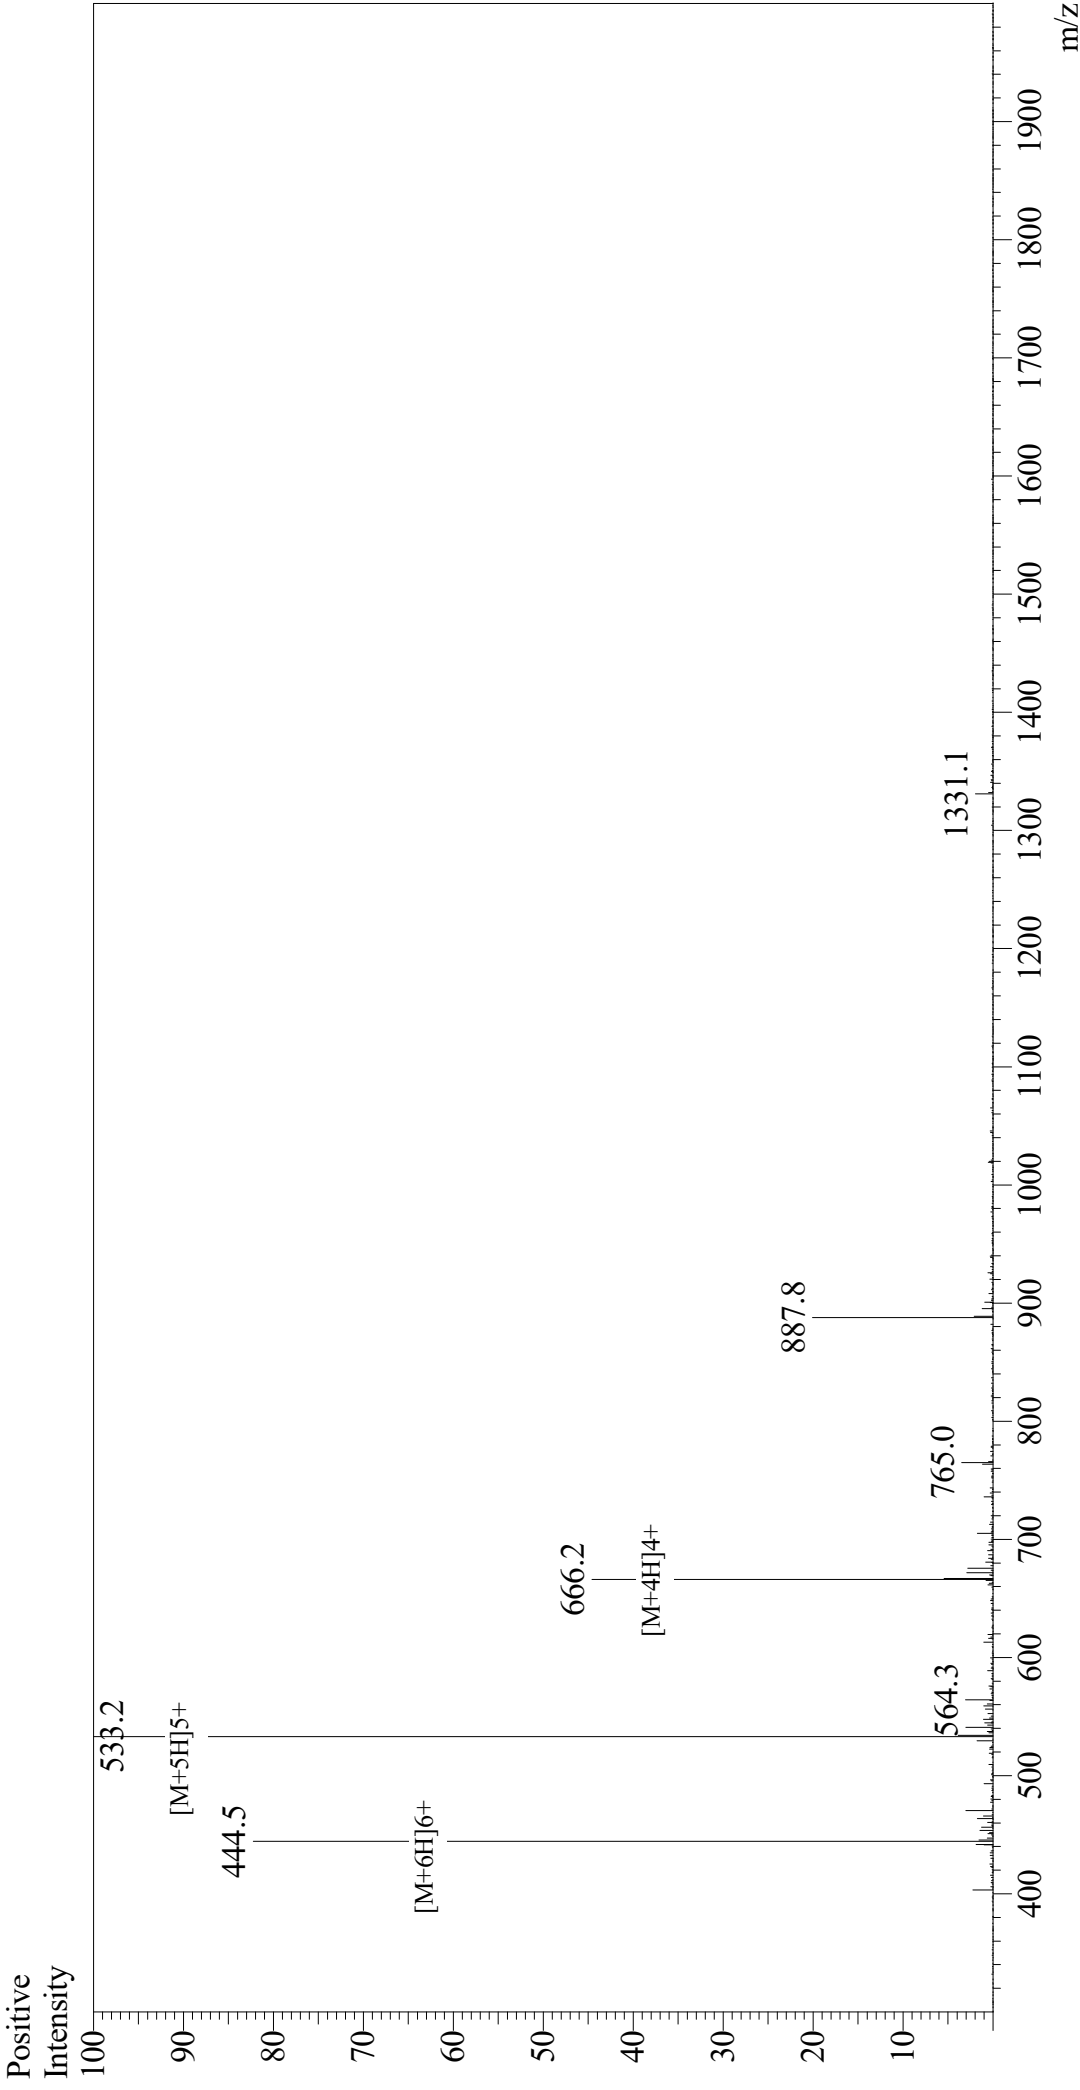

Sample Information

Acquired by : Gary
 Month-Day Processed : 10/14/19
 Time Processed : 09:07:48 PM
 Injection Volume : 0.3
 Sample Name : β -Melanocyte Stimulating Hormone (MSH), human
 Cat. No.: RP10648
 Lot. No.: E7168619J
 Theoretical MW : 2661.00
 Observed MW : 2661.0

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H_2O /50% MeOH