

Sample Name :mTRP-2(180-188)
 Cat No. : RP20250
 Lot No. :PE6141903
 Time Processed : 0:36:24
 Month-Day-Year Processed : 03/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

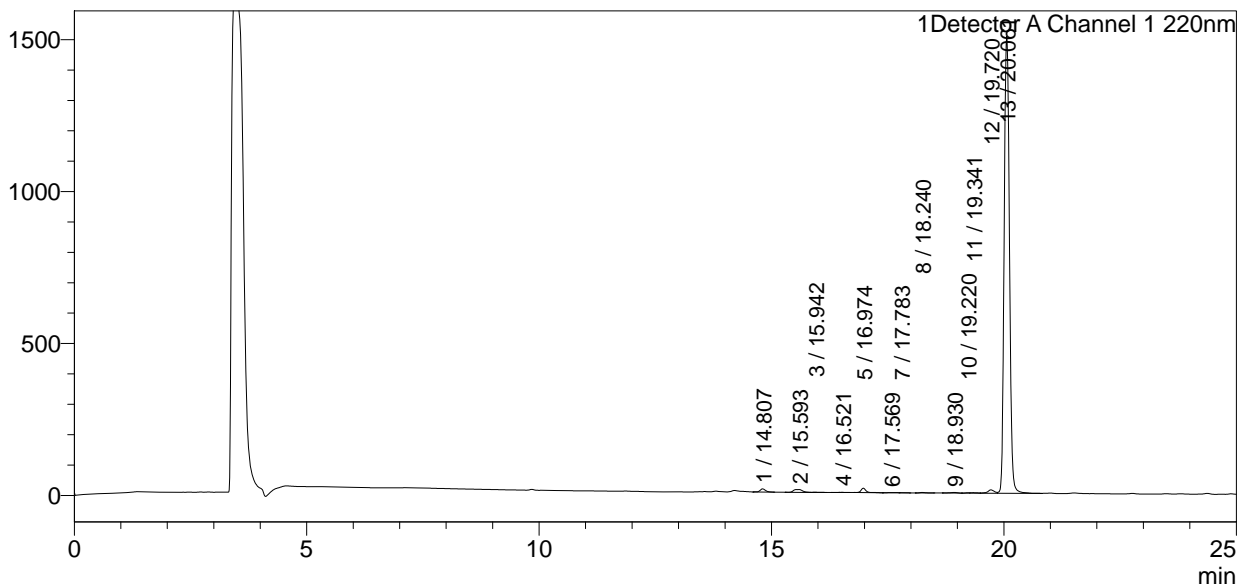

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.807	82756	10497	0.665
2	15.593	124271	9281	0.999
3	15.942	8197	692	0.066
4	16.521	5565	453	0.045
5	16.974	108806	14537	0.875
6	17.569	8339	550	0.067
7	17.783	3600	394	0.029
8	18.240	12051	1623	0.097
9	18.930	22868	1922	0.184
10	19.220	7348	1142	0.059
11	19.341	16803	1571	0.135
12	19.720	108592	11075	0.873
13	20.061	11926387	1503303	95.905
Total		12435582	1557040	100.000