

Sample Name :Cortistatin-14,human,rat
 Cat. No. : RP10972-0.5
 Lot. No. : PE6901710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

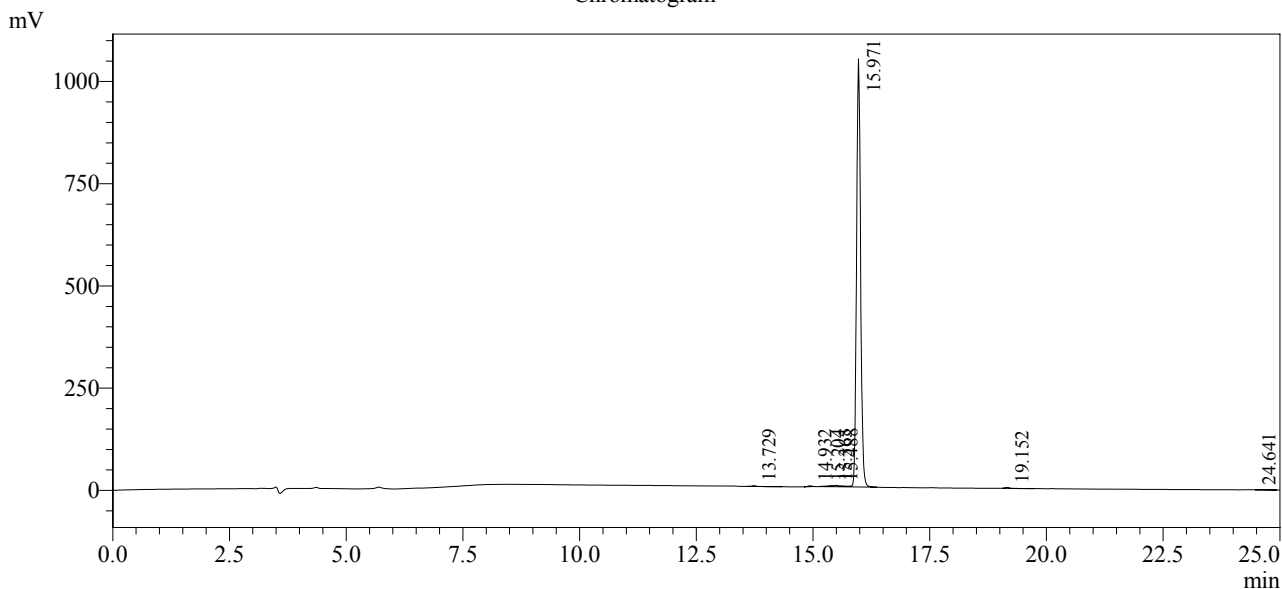

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.729	8417	2036	0.130
2	14.932	11523	1958	0.178
3	15.204	5202	885	0.081
4	15.365	19389	2577	0.300
5	15.488	45306	3210	0.702
6	15.971	6354916	1047115	98.423
7	19.152	8667	2100	0.134
8	24.641	3336	359	0.052
Total		6456758	1060239	100.000