

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E4943220I
 Time Processed :7:20:07 PM
 Month-Day-Year Processed :09/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

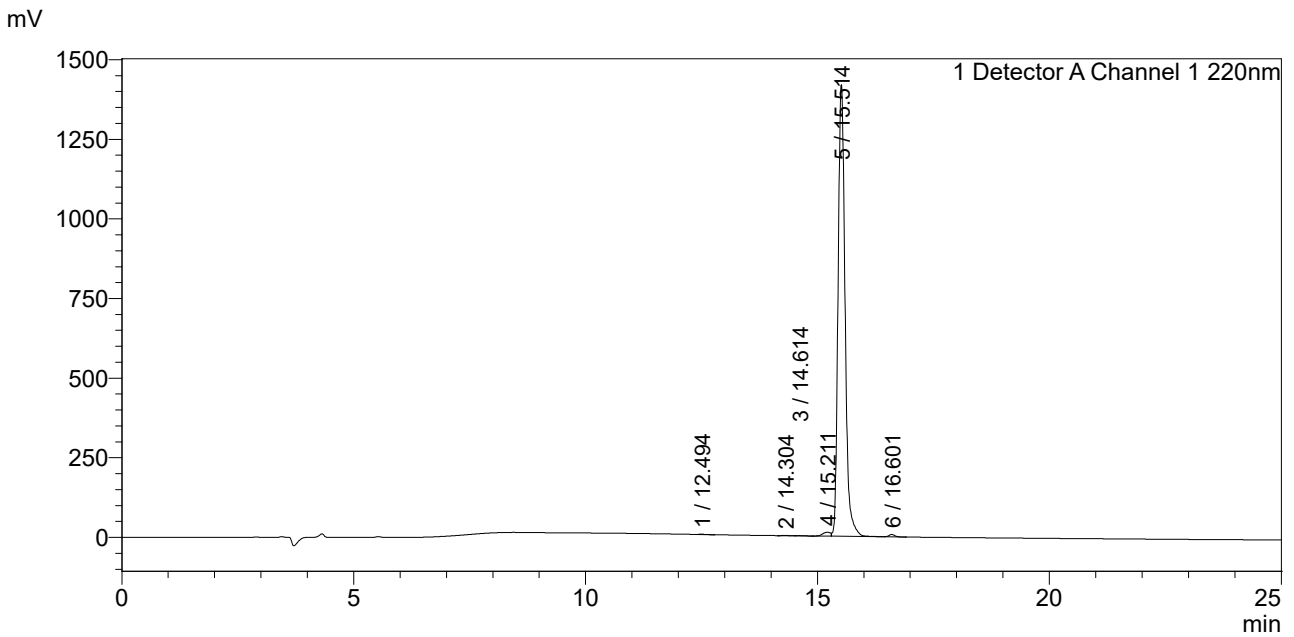

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.494	7588	962	0.050
2	14.304	9148	1068	0.061
3	14.614	7685	1003	0.051
4	15.211	146966	12318	0.977
5	15.514	14812891	1418454	98.451
6	16.601	61708	7404	0.410
Total		15045986	1441208	100.000