


Mass Spectrum

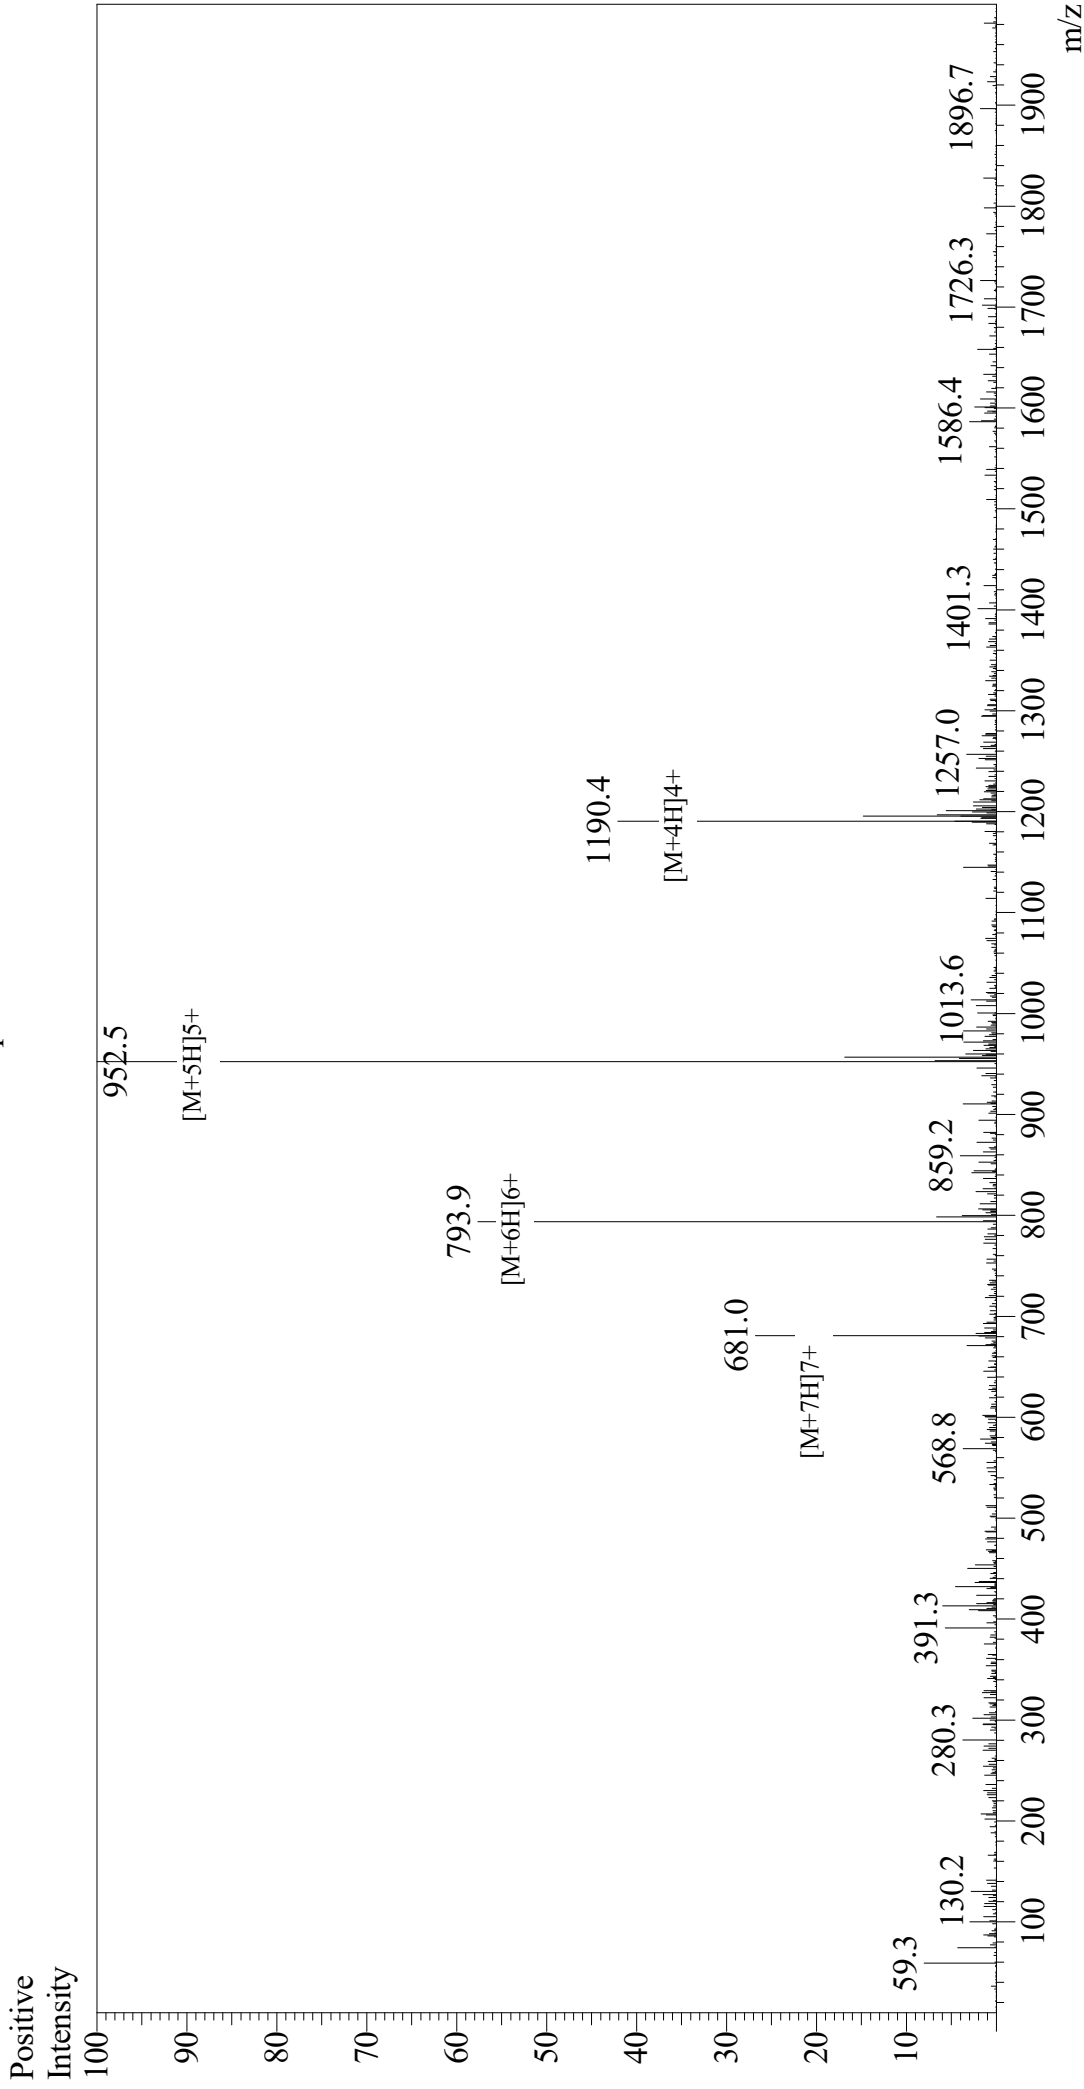

Sample Information

Acquired by : Gary
 Month-Day Processed : 09/30/19
 Time Processed : 04:13:59 PM
 Injection Volume : 0.3
 Sample Name : Corticotropin Releasing Factor, human, rat
 Cat. No. : RP10982
 Lot. No. : E4763319I
 Theoretical MW : 4757.45
 Observed MW : 4757.5

Interface

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H₂O/50%MeOH